

# Minneapolis Blower Door™

## Operation Manual

for

## Model 3 and Model 4 Systems



The **ENERGY**  
**CONSERVATORY**

DIAGNOSTIC TOOLS TO MEASURE BUILDING PERFORMANCE



# Minneapolis Blower Door™

## Operation Manual

### for

## Model 3 and Model 4 Systems

The Energy Conservatory  
2801 21st Ave. S., Suite 160  
Minneapolis, MN 55407  
(612) 827-1117 (Ph)  
(612) 827-1051 (Fax)  
[www.energyconservatory.com](http://www.energyconservatory.com)  
email: [info@energyconservatory.com](mailto:info@energyconservatory.com)

Minneapolis Blower Door, TECTITE, Duct Mask and Automated Performance Testing (APT) System are trademarks of The Energy Conservatory, Inc. Minneapolis Duct Blaster and TrueFlow Air Handler Flow Meter are registered trademarks of The Energy Conservatory, Inc.

Windows and Microsoft Word are registered trademarks of Microsoft Corporation.



Manual Edition: August 2012.

© 2012 by The Energy Conservatory. All rights reserved.

## ENERGY CONSERVATORY WARRANTY

### EXPRESS LIMITED WARRANTY:

Seller warrants that this product, under normal use and service as described in the operator's manual, shall be free from defects in workmanship and material for a period of 24 months, or such shorter length of time as may be specified in the operator's manual, from the date of shipment to the Customer.

### LIMITATION OF WARRANTY AND LIABILITY:

This limited warranty set forth above is subject to the following exclusions:

- a) With respect to any repair services rendered, Seller warrants that the parts repaired or replaced will be free from defects in workmanship and material, under normal use, for a period of 90 days from the date of shipment to the Purchaser.
- b) Seller does not provide any warranty on finished goods manufactured by others. Only the original manufacturer's warranty applies.
- c) Unless specifically authorized in a separate writing, Seller makes no warranty with respect to, and shall have no liability in connection with, any goods which are incorporated into other products or equipment by the Purchaser.
- d) All products returned under warranty shall be at the Purchaser's risk of loss. The Purchaser is responsible for all shipping charges to return the product to The Energy Conservatory. The Energy Conservatory will be responsible for return standard ground shipping charges. The Customer may request and pay for the added cost of expedited return shipping.

The foregoing warranty is in lieu of all other warranties and is subject to the conditions and limitations stated herein. No other express or implied warranty IS PROVIDED, AND THE SELLER DISCLAIMS ANY IMPLIED WARRANTY OF FITNESS for particular purpose or merchantability.

The exclusive remedy of the purchaser FOR ANY BREACH OF WARRANTY shall be the return of the product to the factory or designated location for repair or replacement, or, at the option of The Energy Conservatory, refund of the purchase price.

The Energy Conservatory's maximum liability for any and all losses, injuries or damages (regardless of whether such claims are based on contract, negligence, strict liability or other tort) shall be the purchase price paid for the products. In no event shall the Seller be liable for any special, incidental or consequential damages. The Energy Conservatory shall not be responsible for installation, dismantling, reassembly or reinstallation costs or charges. No action, regardless of form, may be brought against the Seller more than one year after the cause of action has accrued.

The Customer is deemed to have accepted the terms of this Limitation of Warranty and Liability, which contains the complete and exclusive limited warranty of the Seller. This Limitation of Warranty and Liability may not be amended or modified, nor may any of its terms be waived except by a writing signed by an authorized representative of the Seller.

**TO ARRANGE A REPAIR:** Please call The Energy Conservatory at 612-827-1117 before sending any product back for repair or to inquire about warranty coverage. All products returned for repair should include a return shipping address, name and phone number of a contact person concerning this repair, and the purchase date of the equipment.



# **Table of Contents**

<b>SAFETY INFORMATION</b>	<b>1</b>
<b>CHAPTER 1 INTRODUCTION</b>	<b>2</b>
<b>1.1 What is a Blower Door?</b>	<b>2</b>
<b>1.2 Air Leakage Basics</b>	<b>3</b>
1.2.a Stack Effect:	4
1.2.b Wind Pressure:	4
1.2.c Point Source Exhaust or Supply Devices:	4
1.2.d Duct Leakage to the Outside:	4
1.2.e Door Closure Coupled with Forced Air Duct Systems:	4
<b>1.3 Common Air Leakage Sites</b>	<b>4</b>
<b>CHAPTER 2 SYSTEM COMPONENTS</b>	<b>7</b>
<b>2.1 Blower Door Fan</b>	<b>7</b>
2.1.a Determining Fan Flow and Using the Flow Rings:	8
<b>2.2 Test Instrumentation (Pressure and Fan Flow Gauges)</b>	<b>9</b>
2.2.a DG-700 and DG-3 Digital Pressure Gauges:	9
2.2.b Automated Performance Testing System™:	10
<b>2.3 Fan Speed Controllers</b>	<b>11</b>
<b>2.4 Adjustable Aluminum Door Frame</b>	<b>11</b>
<b>2.5 TECTITE Blower Door Test Software</b>	<b>12</b>
2.5.a TECTITE Features:	12
<b>CHAPTER 3 INSTALLING THE BLOWER DOOR FOR DEPRESSURIZATION TESTING</b>	<b>13</b>
<b>3.1 Door Frame and Panel Installation</b>	<b>13</b>
3.1.a Where To Install The Door Frame?	13
3.1.b Installing the Aluminum Frame:	13
<b>3.2 Installing the Outside Building Pressure Tubing</b>	<b>14</b>
<b>3.3 Installing the Blower Door Fan</b>	<b>15</b>
<b>3.4 Attaching the Gauge Mounting Board</b>	<b>15</b>
<b>3.5 Gauge Tubing Connections for Depressurization Testing</b>	<b>16</b>
3.5.a DG-700 Gauge:	16
3.5.b DG-3 Gauge:	16
3.5.c APT System:	17
<b>3.6 Electrical and Tubing Connections to the Fan</b>	<b>17</b>
3.6.a Electrical Connections:	17
3.6.b Connecting Tubing to the Model 3 Fan:	18
3.6.c Connecting Tubing to the Model 4 Fan:	18
<b>3.7 Fan Control Cable for Cruise Control</b>	<b>18</b>
<b>CHAPTER 4 SETTING UP THE BUILDING FOR TESTING</b>	<b>19</b>
<b>4.1 Adjustable Openings</b>	<b>19</b>
<b>4.2 Combustion Appliance/Exhaust Devices</b>	<b>19</b>
<b>4.3 Testing For New Construction</b>	<b>20</b>

<b>CHAPTER 5</b>	<b>CONDUCTING A BLOWER DOOR DEPRESSURIZATION TEST</b>	<b>21</b>
5.1	Choosing a Test Procedure	21
5.2	Depressurization Test Procedures Using the DG-700	21
5.3	Depressurization Test Procedures Using the DG-3	24
5.4	Using the Can't Reach 50 Factors ( <i>One-Point Tests</i> )	27
5.4.a	Potential Errors In One-Point CFM50 Estimate from Using the CRF Factors:	28
5.5	Unable to Reach a Target Building Pressure During a Multi-Point Test?	29
5.6	Testing in Windy Weather	29
5.7	Before Leaving the Building	29
<b>CHAPTER 6</b>	<b>BASIC TEST RESULTS</b>	<b>30</b>
6.1	Basic Airtightness Test Results	30
6.1.a	Air Leakage at 50 Pascals:	30
6.1.b	Normalizing Air Leakage for the Size of the House:	31
6.2	Optional Correction for Air Density	32
6.3	Additional Test Result Options (requires use of TECTITE software)	33
6.3.a	Leakage Areas:	33
6.3.b	Estimated Natural Infiltration Rates:	33
6.3.c	Mechanical Ventilation Guideline:	34
6.3.d	Estimated Cost of Air Leakage:	35
<b>CHAPTER 7</b>	<b>PRESSURIZATION TESTING</b>	<b>36</b>
7.1	Gauge Set-Up For Pressurization Measurements	36
7.1.a	DG-700 and DG-3 Gauges:	36
7.1.b	APT System:	37
7.2	Fan Set-Up For Pressurization Measurements	38
7.3	Optional Correction for Air Density	38
<b>CHAPTER 8</b>	<b>FINDING AIR LEAKS</b>	<b>39</b>
8.1	Using Your Hand	39
8.2	Using a Chemical Smoke Puffer	39
8.3	Using an Infrared Camera	39
8.4	Diagnosing Series Leakage Paths	40
<b>CHAPTER 9</b>	<b>TESTING FOR DUCT LEAKAGE AND PRESSURE IMBALANCES</b>	<b>41</b>
9.1	Duct Leakage Basics	41
9.1.a	Why Is Duct Leakage Important?	41
9.1.b	Where Does Duct Leakage Occur?	41
9.1.c	How Much Can Energy Bills Be Reduced By Sealing Duct Leaks?	42
9.1.d	Duct Leakage to the Outside:	42
9.1.e	Duct Leakage to the Inside:	43
9.2	Finding Duct Leaks to the Outside	43
9.2.a	Smoke Test:	43
9.2.b	Pressure Pan:	43
9.3	Estimating Duct Leakage to the Outside With a Blower Door	44
9.3.a	Modified Blower Door Subtraction:	44

9.3.b Flow Hood Method: (Requires use of calibrated flow capture hood)	46
<b>9.4 Unconditioned Spaces Containing Ductwork</b>	<b>46</b>
<b>9.5 Testing for Pressure Imbalances Caused By Forced Air System Flows</b>	<b>47</b>
9.5.a Dominant Duct Leak Test:	47
9.5.b Master Suite Door Closure:	48
9.5.c All Interior Doors Closed:	48
9.5.d Room to Room Pressures:	49
<b>9.6 Other Important Test Procedures</b>	<b>49</b>
9.6 a Total System Air Flow:	49
9.6.b System Charge:	49
9.6.c Airflow Balancing:	49
<b>CHAPTER 10 COMBUSTION SAFETY TEST PROCEDURE</b>	<b>50</b>
<b>10.1 Overview</b>	<b>50</b>
<b>10.2 Test Procedures</b>	<b>51</b>
10.2.a Measure Ambient CO Level in Building:	52
10.2.b Survey of Combustion Appliances:	52
10.2.c Survey of Exhaust Fans:	52
10.2.d Measure Worst Case Fan Depressurization:	52
10.2.e Spillage Test (natural draft and induced draft appliances):	54
10.2.f Carbon Monoxide Test:	55
10.2.g Draft Test (natural draft appliances):	55
10.2.h Heat Exchanger Integrity Test (Forced Air Only):	55
<b>APPENDIX A CALIBRATION AND MAINTENANCE</b>	<b>57</b>
<b>A.1 Fan Calibration Parameters (Updated January 2007)</b>	<b>57</b>
Model 3 (110V) Calibration Parameters:	57
Model 3 (230V) Calibration Parameters:	57
Model 4 (230V) Calibration Parameters:	57
<b>A.2 Issues Affecting Fan Calibration</b>	<b>58</b>
A.2.a Fan Sensor and Motor Position:	58
A.2.b Upstream Air Flow Conditions:	60
A.2.c Operating Under High Backpressure Conditions:	60
<b>A.3 Blower Door Fan Maintenance and Safety</b>	<b>61</b>
A.3.a Maintenance Checks:	61
A.3.b General Operational Notes and Tips:	61
A.3.c Replacing the Model 4 Controller's Internal Fuse:	61
<b>A.4 Calibration and Maintenance of Digital Pressure Gauges</b>	<b>63</b>
A.4.a Digital Gauge Calibration:	63
A.4.b Digital Gauge Maintenance:	64
<b>A.5 Checking for Leaky Tubing</b>	<b>64</b>
<b>APPENDIX B FLOW CONVERSION TABLES</b>	<b>65</b>
<b>Model 3 (110V)</b>	<b>65</b>
<b>Model 3 (230V)</b>	<b>67</b>
<b>Model 4 (230V)</b>	<b>69</b>

<b>APPENDIX C</b>	<b>USING FLOW RINGS C, D AND E</b>	<b>71</b>
<b>C.1</b>	<b>Using Ring C</b>	<b>71</b>
C.1.a	Installation:	71
C.1.b	Calibration Parameters for Ring C (Updated January 2007):	71
<b>C.2</b>	<b>Using Rings D and E</b>	<b>71</b>
C.2.a	Installation:	71
C.2.b	Measuring Fan Flow with Rings D and E:	72
C.2.c	Calibration Parameters for Rings D and E (Updated January 2007):	72
<b>APPENDIX D</b>	<b>SAMPLE TEST FORMS</b>	<b>74</b>
<b>APPENDIX E</b>	<b>HOME ENERGY ARTICLE *</b>	<b>77</b>
<b>APPENDIX F</b>	<b>CALCULATING A DESIGN AIR INFILTRATION RATE</b>	<b>83</b>
<b>APPENDIX G</b>	<b>REFERENCES</b>	<b>85</b>
<b>APPENDIX H</b>	<b>AIR DENSITY CORRECTION FACTORS</b>	<b>86</b>
H.1	Air Density Correction Factors for Depressurization Testing	86
H.2	Air Density Correction Factors for Pressurization Testing	87
<b>APPENDIX I</b>	<b>CRUISE CONTROL WITH THE DG-700 GAUGE</b>	<b>88</b>
<b>APPENDIX J</b>	<b>BLOWER DOOR SYSTEM SPECIFICATIONS</b>	<b>90</b>

## Safety Information



The Blower Door fan should only be connected to a properly installed and tested power supply. In case of emergencies, disconnect the power cord from the AC power mains outlet. During installation, use the nearest readily accessible power outlet and keep all objects away from interfering with access to the outlet.

- Disconnect the power plug from the Blower Door fan receptacle before examining or making any adjustments to the fan motor, blades or electrical components.
- The Blower Door Fan is a very powerful and potentially dangerous piece of equipment if not used and maintained properly. Carefully examine the fan before each use. If the fan housing, fan guards, blade, controller or cords become damaged, do not operate the fan until repairs have been made. Repairs should only be made by qualified repair personnel.
- If you notice any unusual noises or vibrations, stop and unplug the fan. If you can't find the source of the problem, contact the manufacturer/distributor.
- Keep people, animals and objects away from the Blower Door fan when it is operating.
- Press the power plug firmly into the power receptacle on the Blower Door fan, and the AC power mains outlet. Failure to do so can cause overheating of the power cord and possible damage.
- Do not use ungrounded outlets or adapter plugs. Never remove or modify the grounding prong. Use only approved and inspected electrical wiring and connections.
- Do not operate the Blower Door fan if the motor, controller or any of the electrical connections are wet.
- For long-term operation, such as maintaining building pressure while air-sealing, use a flow ring whenever possible to ensure proper cooling of the BlowerDoor fan motor. This will minimize the heating of the fan and is important in warmer weather.
- Do not reverse the Blower Door fan (if the fan has a flow direction switch) while the blades are turning.
- The motor is thermally protected and if you experience a motor shut down, be sure to turn off the fan speed controller so that the fan does not restart unexpectedly after the motor cools down.
- The operator should wear hearing protection when in close proximity to the fan operating at high speed.
- Adjust all combustion appliances so they do not turn on during the test. If combustion appliances turn on during a depressurization test, it is possible for flames to be sucked out of the combustion air inlet (flame rollout). This is a fire hazard and can possibly result in high CO levels.
- If there are attached spaces (e.g. townhouses) that could contain a vented combustion appliance, either adjust those appliances to prevent them from turning on during the test, or be sure that the attached spaces are not depressurized or pressurized when the Blower Door is operating.
- Be sure that fires in fireplaces and woodstoves are completely out before conducting a test. Take precautions to prevent ashes from being sucked into the building during the test. In most cases it will be necessary to either tape doors shut, clean out the ashes, and/or cover the ashes with newspaper.
- Be sure you have returned the building to its original condition before leaving. This includes turning the thermostat and water heater temperature controls to their original setting. Always check to see that furnace, water heater and gas fireplace pilot lights have not been blown out during the Blower Door test - re-light them if necessary. Remove any temporary seals from fireplaces or other openings sealed during the test.
- If combustion safety problems are found, tenants and building owners should be notified immediately and steps taken to correct the problem including notifying a professional heating contractor if basic remedial actions are not available. Remember, the presence of elevated levels of carbon monoxide in ambient building air or in combustion products is a potentially life threatening situation. Air sealing work should not be undertaken until existing combustion safety problems are resolved, or unless air sealing is itself being used as a remedial action.

## Chapter 1 Introduction


### 1.1 What is a Blower Door?

The Blower Door is a diagnostic tool designed to measure the airtightness of buildings and to help locate air leakage sites. Building airtightness measurements are used for a variety of purposes including:

- Documenting the construction airtightness of buildings.
- Estimating natural infiltration rates in houses.
- Measuring and documenting the effectiveness of airsealing activities.
- Measuring duct leakage in forced air distribution systems.


The Blower Door consists of a powerful, calibrated fan that is temporarily sealed into an exterior doorway. The fan blows air into or out of the building to create a slight pressure difference between inside and outside. This pressure difference forces air through all holes and penetrations in the exterior envelope. By simultaneously measuring the air flow through the fan and its effect on the air pressure in the building, the Blower Door system measures the airtightness of the entire building envelope. The tighter the building (e.g. fewer holes), the less air you need from the Blower Door fan to create a change in building pressure.

Figure 1: Blower Door Depressurization Test

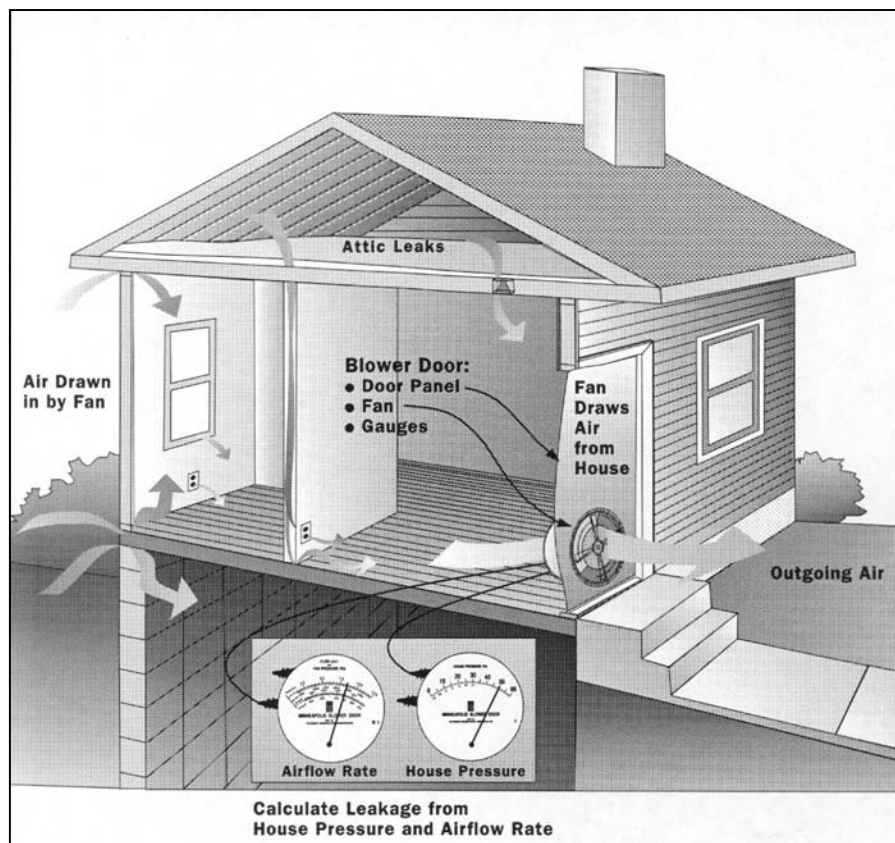

A typical Blower Door test will include a series of fan flow measurements at a variety of building pressures ranging from 60 Pascals to 15 Pascals (one Pascal (Pa) equals approximately 0.004 inches of water column). Tests are conducted at these relatively high pressures to mitigate the effects of wind and stack effect pressures on the test results. Sometimes a simple “one-point” test is conducted where the building is tested at a single pressure (typically 50 Pascals). This is done when a quick assessment of airtightness is needed, and there is no need to calculate leakage areas (i.e. estimate the cumulative size of the hole in the building envelope).

Figure 2: Graph of Blower Door Test Data

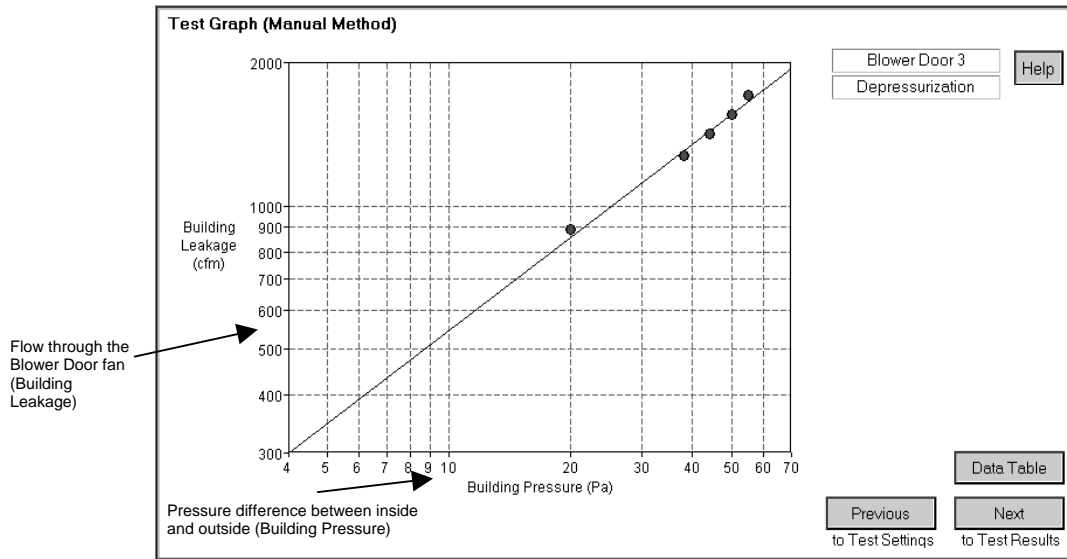

It takes about 20 minutes to set-up a Blower Door, conduct a test, and document the airtightness of a building. In addition to assessing the overall airtightness level of the building envelope, the Blower Door can be used to estimate the amount of leakage between the conditioned space of the building and attached structural components such as garages, attics and crawlspaces. It can also be used to estimate the amount of outside leakage in forced air duct systems. And because the Blower Door forces air through all holes and penetrations that are connected to outside, these problem spots are easier to find using chemical smoke, an infrared camera or simply feeling with your hand. The airtightness measurement can also help you assess the potential for backdrafting of natural draft combustion appliances by exhaust fans and other mechanical devices, and help determine the need for mechanical ventilation in the house.

## 1.2 Air Leakage Basics

To properly utilize the diagnostic capabilities of your Blower Door, it is important to understand the basic dynamics of air leakage in buildings. For air leakage (infiltration or exfiltration) to occur, there must be both a hole or crack, and a driving force (pressure difference) to push the air through the hole. The five most common driving forces which operate in buildings are:

### ***1.2.a Stack Effect:***

Stack effect is the tendency for warm buoyant air to rise and leak out the top of the building and be replaced by colder outside air entering the bottom of the building (**note:** when outside air is warmer than inside air, this process is reversed). In winter, the stack effect creates a small positive pressure at the top of the building and small negative pressures at the bottom of the building. Stack effect pressures are a function of the temperature difference between inside and outside, the height of the building, and are strongest in the winter and very weak in the summer. Stack induced air leakage accounts for the largest portion of infiltration in most buildings.

### ***1.2.b Wind Pressure:***

Wind blowing on a building will cause outside air to enter on the windward side of the building, and building air to leak out on the leeward side.. At exposed sites in windy climates, wind pressure can be a major driving force for air leakage.

### ***1.2.c Point Source Exhaust or Supply Devices:***

Chimneys for combustion appliances and exhaust fans (e.g. kitchen and bath fans) push air out of the building when they are operating. Air leaving the building from these devices causes a negative pressure in the building which draws outside air into holes and cracks in the building envelope. Supply fans (e.g. positive pressure ventilation fan) deliver air into the building creating a positive pressure which pushes inside air out of the building through holes and cracks in the building envelope. (The interaction of ventilation fans on building air leakage and pressures is discussed in Chapter 10)

### ***1.2.d Duct Leakage to the Outside:***

Leaks in forced air duct systems (to the outside) create pressures which increase air leakage in buildings. Leaks in supply ducts act like exhaust fans causing negative building pressures. Leaks in return ducts act like supply fans creating positive pressures in buildings. (Duct leakage and duct leakage diagnostics are discussed in more detail in Chapter 9).

### ***1.2.e Door Closure Coupled with Forced Air Duct Systems:***


Research has shown that in buildings with forced air duct systems, imbalances between supply and return ducts can dramatically increase air leakage. For example, a study conducted in Florida showed that infiltration rates in many houses were doubled whenever the HVAC system fan was operating due to pressures caused by door closure. In the Florida houses, closing of bedroom doors created large duct imbalances by effectively cutting off the bedroom supply registers from the central return registers located in the main part of the house. (Duct leakage and duct leakage diagnostics are discussed in more detail in Chapter 9)

## **1.3 Common Air Leakage Sites**

Common air leakage sites are shown in Figure 3 below. Notice how as warm air rises due to the stack effect, it tends to escape through cracks and holes near the top of the building. This escaping air causes a slight negative pressure at the bottom of the building which pulls in cold air through holes in the lower level. Air sealing activities should usually begin at the top of the building because this is where the largest positive pressures exist and where many of the largest leakage sites (and potential condensation problems) can be found.

The next most important location of leaks is in the lowest part of the building. The bottom of the building is subject to the largest negative pressures, which induces cold air infiltration. Importantly, if spillage prone natural draft combustion appliances are present, do not seal lower level building leaks unless you have first addressed leaks in the attic or top part of the building. Sealing only lower level leakage areas while leaving large high level leaks could create large enough negative pressures to cause combustion appliance backdrafting.

Figure 3: Common Air Leakage Sites

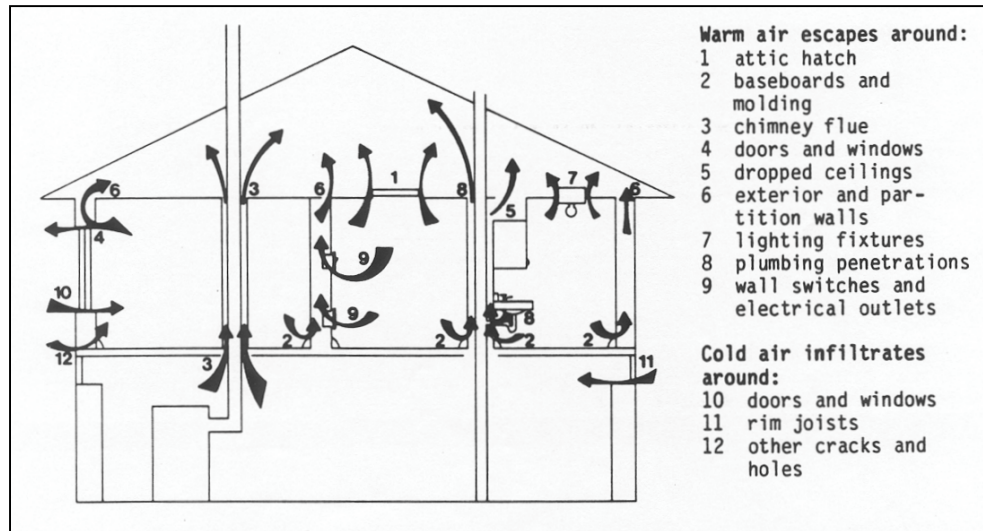

In addition to these common leakage sites, there can also be large leakage paths associated with hidden construction details such as attached porches, cantilevered floors and overhangs. Figures 4 - 6 show a number of potentially important leakage paths which are often overlooked by crews using traditional weatherization techniques. Use of densely blown cellulose insulation or other barrier-type air sealing techniques at these key junctures often result in dramatic air leakage reductions.

Figure 4: Hidden Construction Details

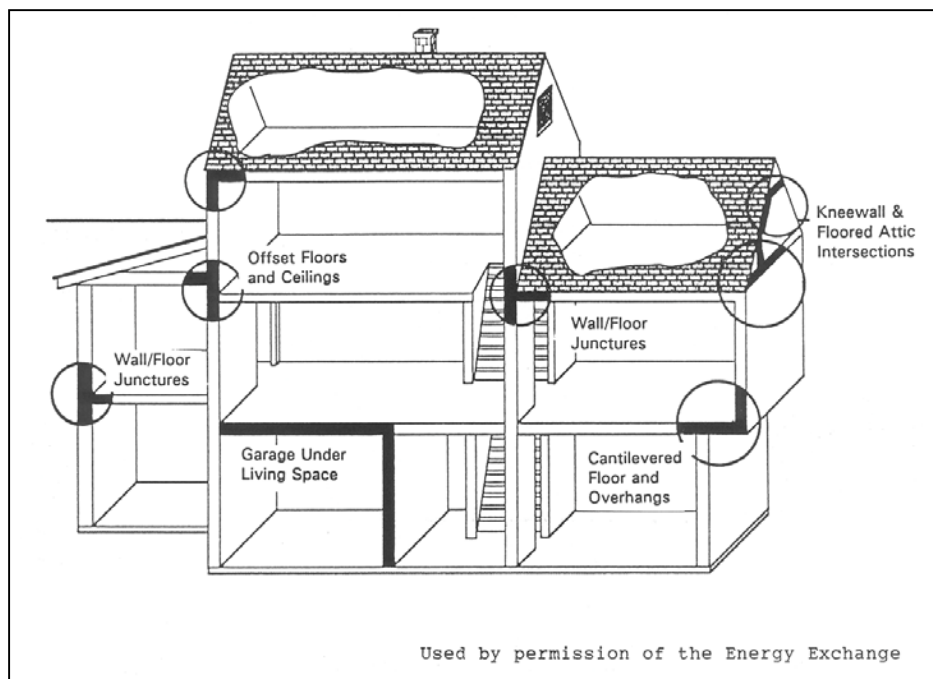


Figure 5: Leak from Attached Porch


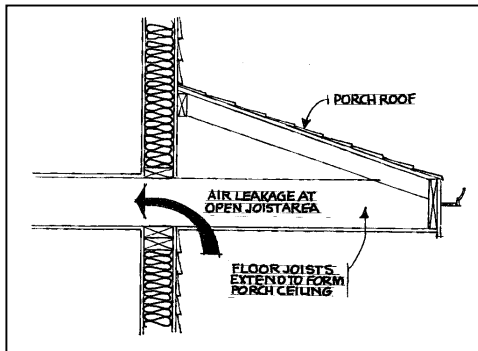


Figure 6: Common Kneewall Leak

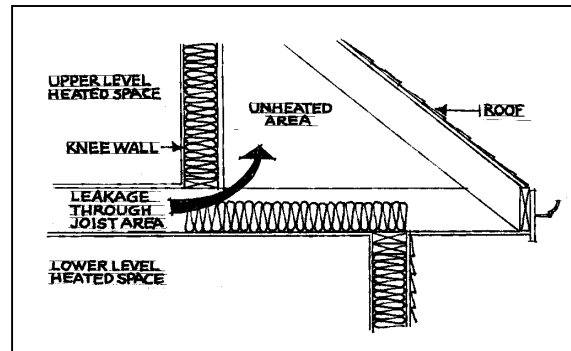

Forced air system ductwork can also be a major air leakage site. Even small leaks in ductwork can result in significant air leakage due to the high pressures found in ducts whenever the heating or cooling system is operating. More information on duct leakage can be found in Chapter 9.

## Chapter 2 System Components

This Manual includes operating instructions for the following models of Minneapolis Blower Door:

- Model 3/110V System
- Model 3/230 System
- Model 4/230V System (CE labeled fan and controller)

Both the Model 3 and Model 4 Minneapolis Blower Door systems are comprised of three separate components:

1. Blower Door Fan
2. Accessory Case with Test Instrumentation (building pressure and fan flow gauges), Fan Speed Controller and Nylon Door Panel
3. The Adjustable Aluminum Door Frame



While the Blower Door fan motor, flow sensor and speed controller vary slightly between the three different Minneapolis Blower Door systems, the other system components are identical.

PC based test analysis software (TECTITE™) is also available to help you document and analyze Blower Door test results.

### **2.1 Blower Door Fan**

The Blower Door fan consists of a molded fan housing with a 3/4 h.p. permanent split capacitor AC motor. Air flow through the fan is determined by measuring the pressure at the flow sensor which is attached to the end of the motor. When the fan is operating, air is pulled into the inlet side of the fan and exits through the exhaust side (a metal fan guard is bolted to the exhaust side of the fan).


The Blower Door fan can accurately measure airflow over a wide range of flow rates using a series of calibrated Flow Rings which are attached to the inlet of the fan. The standard Minneapolis Blower Door system comes with 2 Flow Rings (A and B) capable of measuring flows as low as 300 Cubic Feet per Minute (cfm). Optional Rings C, D and E are available which allows flow measurements as low as 85, 30 and 11 cfm respectively.

Model 3 Fan with Rings A and B




The main distinguishing feature between the Model 3 and Model 4 fans is the shape of the flow sensor attached to the fan motor. Model 3 fans (both 110V and 230V) use a round white plastic flow sensor, while the Model 4 fan uses a flow sensor manufactured out of stainless steel tubing.

Model 3 Fan and Flow Sensor

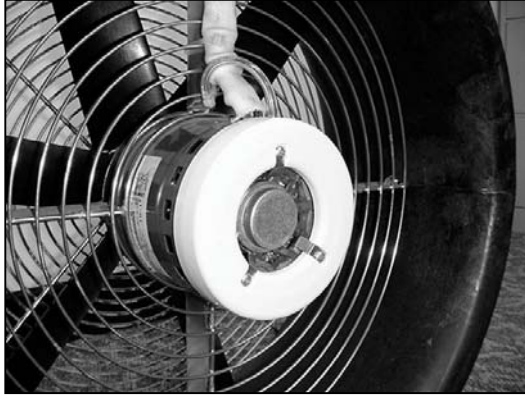

Model 4 Fan and Flow Sensor

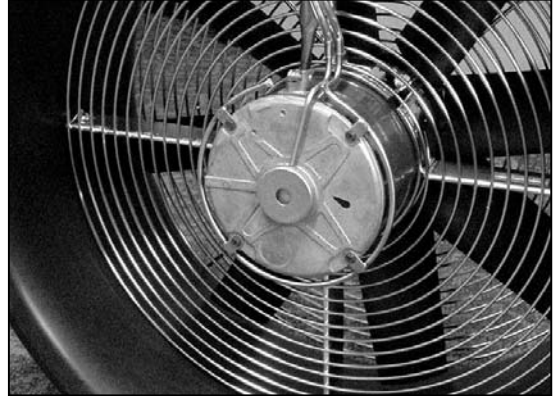

### 2.1.a Determining Fan Flow and Using the Flow Rings:

Fan pressure readings from the flow sensor are easily converted to fan flow readings by using a Flow Conversion Table (see Appendix B), by reading flow directly from the Blower Door gauge(s), or through the use of the TECTITE Blower Door Test Analysis Software. The Blower Door fan has 6 different flow capacity ranges depending on the configuration of Flow Rings on the fan inlet. Table 1 below show the approximate flow range of the Blower Door fan under each of the 6 inlet configuration. The greatest accuracy in fan flow readings will always be achieved by installing the Flow Ring with the smallest opening area, while still providing the necessary fan flow. Importantly, when taking Blower Door measurements, stand at least 12 inches from the side of the fan inlet. Standing directly in front of the fan may affect the flow readings and result in erroneous measurements.

Table 1: Fan Flow Ranges

Fan Configuration	Flow Range (cfm) for Model 3 Fan	Flow Range (cfm) for Model 4 Fan
Open (no Flow Ring)	6,100 - 2,435	4,850 - 2,090
Ring A	2,800 - 915	2,500 - 790
Ring B	1,100 - 300	900 - 215
Ring C	330 - 85	260 - 45
Ring D	115 - 30	125 - 30
Ring E	45 - 11	50 - 11

To install **Flow Ring A**, place Ring A onto the inlet side of the fan housing and rotate the 8 fastener clips attached to the housing flange so that they rotate over the edge of Ring A and secure it in place.



To Install **Flow Ring B**, place Ring B in the center of Ring A and rotate the 6 fastener clips attached to Ring A so that they rotate over the edge of Ring B and secure it in place.



In addition to Flow Rings A and B, the standard Minneapolis Blower Door comes with a solid circular **No-Flow Plate** to seal off the fan opening. The No-Flow Plate is attached to Ring B in the same manner that Ring B attaches to Ring A.

The No-Flow Plate and Rings A and B can be removed separately, or all 3 pieces can be removed at the same time by releasing the 8 fastener clips holding Ring A to the fan housing.

Installation and use of optional Flow Rings C, D and E are discussed in Appendix C.



## **2.2 Test Instrumentation (Pressure and Fan Flow Gauges)**

This manual covers three instrumentation options typically used with the Minneapolis Blower Door; the DG-700 Digital Gauge, the DG-3 Digital Gauge, and the APT System.

### ***2.2.a DG-700 and DG-3 Digital Pressure Gauges:***

The DG-700 and DG-3 are differential pressure gauges which measure the pressure difference between either of their **Input** pressure taps and its corresponding bottom **Reference** pressure tap. Both gauges have two separate measurement channels which allows you to monitor the building pressure and fan pressure (air flow) signals during the Blower Door test (the DG-700 allows for simultaneous display of both channels, while the DG-3 can display one channel at a time). In addition, both gauges are able to directly display air flow through the Blower Door fan (the DG-700 can display fan flow in units of cfm, l/s and m<sup>3</sup>/hr). The digital gauge is shipped in a separate padded case which is stored in the Blower Door accessory case. Also included is a black mounting board to which the digital gauge can be attached using the Velcro strips found on the back of the gauge.

The DG-700 can also be used to automate control of the Blower Door fan using the following two features:

- The-DG-700 can be used along with TECTITE software and a user supplied laptop computer to conduct a fully automated Blower Door test. When conducting automated tests, the speed of the Blower Door fan is computer controlled while the TECTITE program simultaneously monitors the building pressure and fan flow using the DG-700's two pressure channels. Test results are recorded, displayed on the screen, and can be saved to a file. **Note:** Automated testing requires the TECTITE software and special cabling.
- Newer DG-700 gauges have a built-in "Cruise Control" feature which allow the user to control the Blower Door fan to maintain a constant building pressure, without using the TECTITE software or a laptop computer.

DG-700 Pressure Gauge



DG-3 Pressure Gauge



### 2.2.b Automated Performance Testing System™:

The Automated Performance Testing (APT) system performs fully automated Blower Door tests from a user supplied laptop or desktop computer using TEC's TECTITE software. The TECTITE software allows the user to select among various airtightness testing procedures, including a cruise control option which maintains the building at any user-defined pressure. The APT system automatically adjusts the speed of the Blower Door fan while simultaneously monitoring the building pressure and fan flow using 2 on-board differential pressure channels. Test results are recorded, displayed on the screen, and can be saved to a file.

If the APT system contains more than 2 installed pressure channels, the additional channels can be used to monitor and record pressures in attached zones (e.g. attic or crawlspace) during the automated Blower Door test.

The APT system consists of the following components:

- One Data Acquisition Box (DAB) with 2 to 8 on-board pressure channels and phone jacks for 8 voltage input channels.
- One 6' serial cable (w/ 9 pin connectors) to connect the DAB with your computer.
- One 12V power supply for the DAB.
- One CD containing the TECTITE software.



The Data Acquisition Box (DAB) comes fastened to a black plastic mounting board. The mounting board may also contain two electrical outlets which can be used to power the Blower Door fan, DAB or a lap-top computer.

**Note:** When using an APT system, only automated Blower Door testing can be conducted because the APT's DAB does not have a built-in display. Manual testing must be done with a DG-700 or DG-3 gauge.

## 2.3 Fan Speed Controllers


Model 3 and Model 4 Blower Door fans are supplied with a speed controller. Fan speed is adjusted using the adjustment knob on the face of the speed controller. Model 3 Blower Door systems come with the fan speed controller clipped onto the black mounting board supplied with the system. The Model 3 controller can be removed from the mounting board by sliding the controller clip off the board.

The Model 4 fan speed controller will either be attached to a mounting board (system with DG-700 gauge), or simply have an attachment clamp connected directly on the back of the speed controller box (system with APT system).

**Model 3 Speed Controller**




**Model 4 Speed Controller**

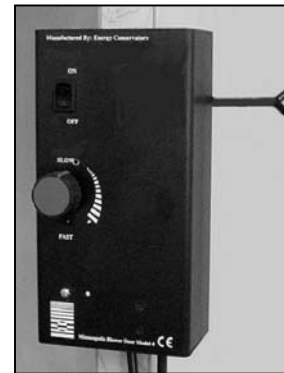

## 2.4 Adjustable Aluminum Door Frame

The adjustable aluminum door frame (and nylon panel) is used to seal the fan into an exterior doorway. The door frame is adjustable to fit any typical size residential door opening. The aluminum frame consists of 5 separate pieces which are shipped in a soft-sided cloth frame case. The two longest frame pieces make up the vertical sides of the door frame, while the two remaining shorter frame pieces make up the top and bottom. The cross bar has a hook on either end of the bar. The frame was designed to be quickly assembled and broken down to simplify storage and transport. If desired, the frame can be transported completely assembled.


To assemble the frame, remove one long and one short frame piece from the case. Disengage the cam levers on each piece by flipping the cam lever to the relaxed position. Be sure the adjustment knobs have been tightened so

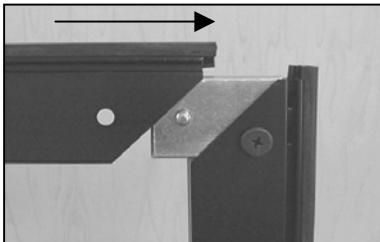

that the frame piece does not extend as you put the frame together. Snap the two pieces together by sliding one end of the short piece over one corner block on the long frame piece. You will need to push in the round bullet on the corner block as you slide the pieces together. The round bullet will snap into the hole located on the short frame piece. Assemble all four sides of the frame together in this manner. Be sure that the cam levers and adjustment knobs are all on the same side of the frame as you assemble the pieces.



Now remove the cross bar from the frame case. The hooks at each end of the middle bar will fit into one set of slots which are found on the inside edges of the vertical frame pieces. To insert the middle frame bar, first loosen the adjustment knobs on the cross bar and the top and bottom frame pieces. With the frame adjusted to its smallest size and the cam levers and knobs facing you, insert one hook into the 2nd slot from the top on one side of the frame. Extend the middle bar and insert the second hook on the other side of the frame. Push the middle bar down so that the hooks are fully set into the slots.

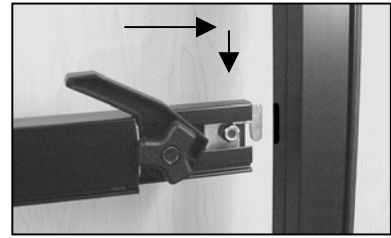

Assembled Aluminum Frame



## **2.5 TECTITE Blower Door Test Software**

TECTITE is a Blower Door test analysis program for PC computers. The TECTITE program can be used to calculate and display airtightness test results from manually collected Blower Door test data. In addition, TECTITE can be used along with a DG-700 gauge or APT System to conduct fully automated building airtightness tests.

### ***2.5.a TECTITE Features:***

- Easy data entry of all test data and building information.
- Calculation and display of airtightness test results including CFM50, air changes per hour, leakage areas, estimated annual and design natural infiltration rates, and estimated cost of air leakage.
- Choice of 4 test standards including CGSB 149.10-M86 and the 3 RESNET test standards.
- Estimates needed mechanical ventilation based on ASHRAE Standard 62.2-10.
- Built-in PDF report generator and compare file features.
- TECTITE lets you print your company logo directly on the reports.
- Compatible with both Model 3 and Model 4 Blower Door Systems.
- Fully automates Blower Door testing when used with a DG-700 gauge or APT system.

**Note:** If you receive the TECTITE software, the program CD contains a separate software operation manual. A fully functional copy of TECTITE is available to download from The Energy Conservatory's website at [www.energyconservatory.com](http://www.energyconservatory.com).

## Chapter 3 Installing the Blower Door for Depressurization Testing

The following instructions are for conducting building **depressurization** tests (i.e. blowing air out of the building). Depressurization testing is the most common method for taking Blower Door measurements.

One of the primary reasons depressurization testing is the most commonly used test method is that back-draft dampers in exhaust fans and dryers will be pulled closed during the test. Because back-draft dampers are typically shut most of the time, leakage from these devices should generally not be included in the results of a Blower Door test.

Information on how and why to conduct Blower Door **pressurization** tests (i.e. blowing air into the building) is discussed in Chapter 7.

### 3.1 Door Frame and Panel Installation

#### 3.1.a Where To Install The Door Frame?

- It is always best to install the Blower Door system in an exterior doorway of a large open room.
- Try to avoid installing the fan in a doorway where there are stairways or major obstructions to air flow very close (1-5 feet) to the fan inlet. See Appendix A for additional information on obstructions to air flow.
- If the doorway leads to a porch or garage, make sure this space is open to the outside by opening doors and/or windows.
- The door frame is almost always installed from the inside of the building and may be installed in place of the prime door, the storm door, or anywhere in between.
- Always open the inside door and outside storm door as much as possible during the test to prevent restrictions to airflow.

#### 3.1.b Installing the Aluminum Frame:

The first step is to fit the adjustable frame loosely in the door opening. Adjust the width of the frame by loosening the three knobs on the top, middle and bottom frame pieces and sliding the sides apart. The side frame weatherstripping should be touching the sides of the door jam opening, but should be easily removed. Retighten the knobs.



Now loosen the knobs on the 2 vertical frame pieces and slide the frame up to the top of the door opening. Retighten the vertical frame piece knobs.



Remove the frame from the door opening and set it up against a wall. Take the nylon panel out of the accessory case and drape the top of the panel over the top of the frame. Use the long Velcro strip at the top of the panel to hold the panel over the top frame piece.




Use the two Velcro tabs at the bottom of the panel to secure the panel around the bottom piece of the frame. Once the bottom tabs are attached, readjust the top Velcro strip to remove any slack and tighten the panel vertically over the frame.



Now pull both sides of the panel tightly around the frame and secure the panel with the 4 side Velcro tabs. The frame and panel should now look like the picture to the right.

You are now ready to fit the frame and panel into the door opening and secure it in place. Lift the frame and panel assembly and insert it into the doorway and up against the door stop. Once the frame is firmly pushed up against the door stop,

release the top Velcro strip and 4 side Velcro tabs. If necessary, re-adjust the frame so it fits snugly in the door opening, being sure to re-tighten the 5 adjustment knobs.

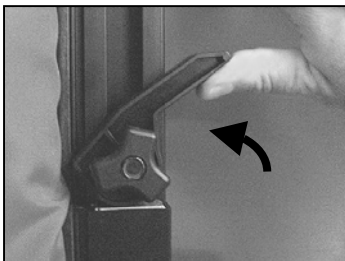

Now engage the five cam levers so that the frame is secured tightly into the opening. These cam levers provide the final tightening in the door opening.


**Note:** If the frame does not fit tightly, disengage the cam levers, re-adjust the frame to fit tighter in the opening, and then re-engage the cam levers.



### 3.2 Installing the Outside Building Pressure Tubing

Run approximately 3 - 5 feet of one end of the **Green** tubing outside through one of the patches in the bottom corners of the nylon panel. Be sure the outside end of the tubing will be placed well away from the exhaust flow of the Blower Door fan.

Outside pressure tubing should be placed away from fan exhaust.

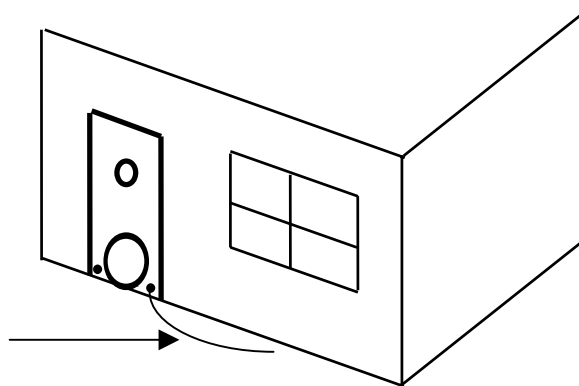

### 3.3 Installing the Blower Door Fan

Place the fan, with the Flow Rings and no-flow plate installed, in line with the large hole in the door panel. The exhaust side of the fan should be facing the door panel. Now tip the fan forward with one hand while you stretch the elastic panel collar over the exhaust flange of the fan. The elastic panel collar should fit snugly around the fan with the collar resting in the gap between the two sides of the electrical box.



The fan is held in place and stabilized by the Velcro strap attached to the aluminum frame cross bar. Slip the Velcro strap through the fan handle and loop it up and back around the cross bar. Pull the strap tight so that it is holding the bottom fan flange off the floor (approximately 2 inches off the floor if possible). The Velcro strap can now be attached to itself.



### 3.4 Attaching the Gauge Mounting Board

The black mounting board for the DG-700, DG-3, or the APT Data Acquisition Box can be attached to any door by using the C-clamp connected to the back of the board. The mounting board can also be easily attached to a horizontal surface (book shelf or desk top) by rotating the clamp 90 degrees before securing the board.



In addition, the mounting board can be attached to the gauge hanger bar which comes with the adjustable aluminum door frame. To use this option, connect the gauge hanger bar to either side of the aluminum frame by inserting the hook into one of the remaining slots on the side of the frame. You can now tighten the mounting board clamp onto the hanger bar.




### 3.5 Gauge Tubing Connections for Depressurization Testing

The Minneapolis Blower Door system comes with 2 pieces of color coded tubing - a 15 foot length of **Green** tubing for measuring building pressure, and a 10 foot length of **Red** tubing to measure fan pressure and flow. Connect the remaining end of the **Green** tubing (the other end should be running outside through the nylon panel) and one end of the **Red** tubing to the gauge(s) as shown below:

#### 3.5.a DG-700 Gauge:

Connect the **Red** tubing to the Channel B Input tap. **Channel B is used to measure Fan pressure and flow.**


Connect the **Green** tubing to the Channel A Reference tap. **Channel A is used to measure building pressure with reference to outside.**

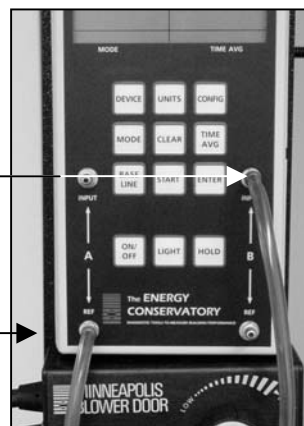

#### 3.5.b DG-3 Gauge:

Connect the **Red** tubing to the Channel B Input tap. **Channel B is used to measure Fan pressure and flow.**

Connect the **Green** tubing to the Channel A Reference tap. **Channel A is used to measure building pressure with reference to outside.**

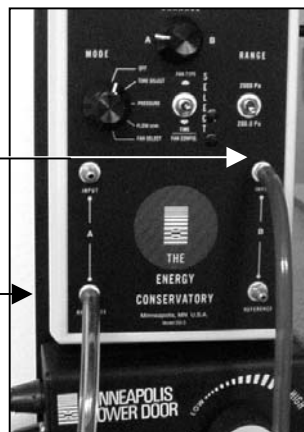

### 3.5.c APT System:

Connect the **Red** tubing to the Channel P2 Input tap. Channel P2 is used to measure fan pressure and flow.

Connect the **Green** tubing to the Channel P1 Reference tap. Channel P1 is used to measure building pressure with reference to outside.


APT-2



Connect the **Red** tubing to the Channel P2 Input tap. Channel P2 is used to measure fan pressure and flow.

Connect the **Green** tubing to the Channel P1 Reference tap. Channel P1 is used to measure building pressure with reference to outside.

APT-3 through 8

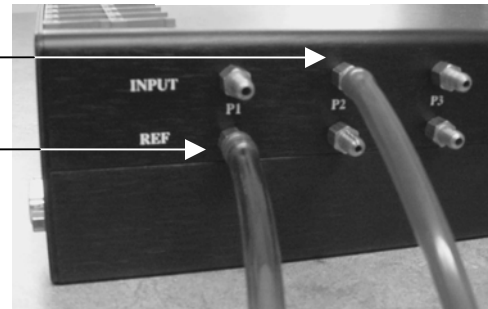

**Note:** See the TECTITE manual for information on measuring zone pressures with installed pressure channels P3 through P8.

## 3.6 Electrical and Tubing Connections to the Fan

### 3.6.a Electrical Connections:



Insert the female plug from the fan speed controller into the receptacle located on the fan electrical box. **Make sure that the plug is pushed completely into the receptacle - overheating of the plug or receptacle can result if not installed correctly.** The remaining cord (power cord) should be plugged into an AC power mains outlet that is compatible with the Voltage of the fan motor and speed controller. Be sure the fan controller knob is turned all the way counter clockwise to the "off" position before plugging into the power outlet.

If you are using an older Model 3 fan, check that the fan direction switch is in the proper position. The fan direction switch (located on the fan electrical box) determines the air flow direction. In order to measure air flow during a Blower Door test, air must flow through the fan inlet and out the exhaust side of the fan.

**Note:** Model 4 fans and newer Model 3 fans are not reversible.



In case of emergencies, disconnect the power cord from the AC power mains outlet. During installation, use the nearest readily accessible power outlet and keep all objects away from interfering with access to the outlet.

### 3.6.b Connecting Tubing to the Model 3 Fan:


The remaining end of the **Red** tubing should now be connected to the single pressure tap on the Model 3 Blower Door fan electrical box (the other end of the **Red** tubing is connected to the Channel B/P2 Input tap).



### 3.6.c Connecting Tubing to the Model 4 Fan:

**Note:** Newer Model 4 fans have 2 pressure taps mounted on the fan electrical box. Older Model 4 fans have a single pressure tap.

Connect the remaining end of the **Red** tubing to this pressure tap (the other end of the **Red** tubing is connected to the Channel B/P2 Input tap).

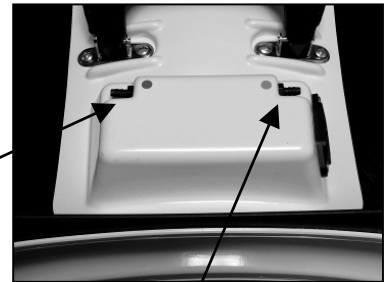

If your Model 4 fan has 2 pressure taps located on the electrical box, connect this second pressure tap (located by the receptacle) to the Channel B/P2 Reference tap using an additional piece of **Clear** tubing provided with your system.


**Note:** Use of this second pressure tap is not required, provided that the Channel B/P2 Reference tap is sensing the air pressure upstream of the fan (i.e. the air being pulled into the fan).

## 3.7 Fan Control Cable for Cruise Control


Beginning June 2007, a Cruise Control feature was added to the DG-700 which allows you to automatically control the Blower Door fan to maintain a constant building pressure, without having the gauge connected to a computer. Common applications of Cruise include conducting a one-point 50 Pa airtightness test and maintaining a constant building pressure for diagnostic procedures (e.g. pressure pan). To use Cruise Control, you must install a fan control cable between the fan control jack on the top of the DG-700 gauge, and the communication jack on the side of the Blower Door fan speed controller (see Appendix I for more information).



Fan control cable.

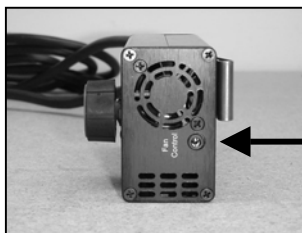

Fan control jacks.

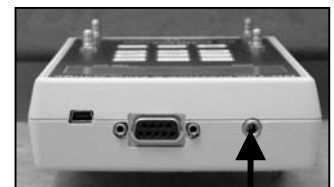

## Chapter 4 Setting Up the Building for Testing

After installing the Blower Door system, you will need to set up the building for the airtightness test. This typically includes closing adjustable openings and preparing combustion appliances and exhaust fans. The following preparations are appropriate when using the Blower Door to determine retrofit airsealing potential, weatherization effectiveness or estimating natural infiltration rates. If the purpose of the Blower Door test is to document construction airtightness quality for new houses, additional preparation may be needed (see Testing For New Construction below). If you are using the Blower Door to estimate duct leakage, see Chapter 9 for set up procedures. Your program guidelines may require you to prepare the building differently than described below.

**Note:** The building set-up and test procedures contained within this manual are recommended specifically by The Energy Conservatory. These procedures generally conform to the Canadian General Standards Board (CGSB) standard CGSB-149.10-M86 "Determination of the Airtightness of Building Envelopes by the Fan Depressurization Method", and American Society for Testing and Materials (ASTM) standard E779-10 "Standard Test Method for Determining the Air Leakage Rate by Fan Pressurization". However, our procedures include options and recommendations that are not contained within the CGSB and ASTM standards. If you need to perform a Blower Door airtightness test that exactly meets the CGSB, ASTM or some other test procedure (e.g. RESNET), you should obtain a copy of the applicable standard and follow the specific set-up directions contained in the standard.

### 4.1 Adjustable Openings

- Close all storm and prime windows.
- Close all exterior doors and interior attic or crawlspace hatches which are connected to conditioned spaces. Also close exterior crawl space hatches and vents if they are normally closed most of the year.
- Open all interior doors to rooms that are conditioned. The object here is to treat the entire building as one conditioned space and to subject all of the leaks in the building to the same pressure difference. Because few house basements can be completely sealed from the house and usually some conditioning of the basement is desirable, they are typically included as conditioned space.
- Tape plastic over window air conditioners if they appear to be a source of air leakage into the building and they are typically removed during a large part of the year.

### 4.2 Combustion Appliance/Exhaust Devices

- Adjust all combustion appliances so they do not turn on during the test. This is commonly done by temporarily turning off power to the appliance, or setting the appliance to the "Pilot" setting. **Note:** *If combustion appliances turn on during a depressurization test, it is possible for flames to be sucked out of the combustion air inlet (flame rollout). This is a fire hazard and can possibly result in high CO levels.*
- If there are attached spaces (e.g. townhouses) that could contain a vented combustion appliance, either adjust those appliances to prevent them from turning on during the test, or be sure that the attached spaces are not depressurized or pressurized when the Blower Door is operating.
- Be sure that fires in fireplaces and woodstoves are completely out. Take precautions to prevent ashes from being sucked into the building during the test. In most cases it will be necessary to either tape doors shut, clean out the ashes, and/or cover the ashes with newspaper.
- Turn off all exhaust fans, vented dryers, air conditioners, ventilation system fans and air handler fans.

### **4.3 Testing For New Construction**

If the Blower Door test is being performed to document performance compliance with building codes, the building should be set-up in accordance with the specific requirements of the applicable building code. For example, the 2012 International Energy Conservatory Code contains the following language in reference to building set-up:

- Exterior windows and doors, fireplace and stove doors should be closed, but not sealed, beyond the intended weatherstripping or other infiltration control measures.
- Dampers including exhaust, intake, makeup air, backdraft and flue dampers shall be closed, but not sealed beyond intended infiltration control measures.
- Interior doors, if installed at the time of the test, shall be open.
- Exterior doors for continuous ventilation systems and heat recovery ventilators shall be closed and sealed.
- Heating and cooling systems, if installed at the time of the test, shall be turned off.
- Supply and return registers, if installed at the time of the test, shall be fully open.

## Chapter 5 Conducting a Blower Door Depressurization Test

The following instructions assume you are conducting a depressurization test and have set up the Blower Door system and building as outlined in Chapters 3 and 4 above. These instructions cover manual test operation using the DG-700 and DG-3 Digital Pressure Gauges. If you are using the DG-700 or APT System to conduct a fully automated Blower Door test with the TECTITE Software, follow the test instructions contained in the TECTITE Software Users Guide (available from the TECTITE Help menu). Information on how and why to conduct Blower Door pressurization tests (i.e. blowing air into the building) is discussed in Chapter 7.

### 5.1 Choosing a Test Procedure

The two most common Blower Door test procedures used to assess overall building airtightness are the *One-Point Test* and the *Multi-Point Test*. The *One-Point Test* utilizes a single measurement of fan flow needed to create a 50 Pascal change in building pressure. The *One-Point Test* provides a quick and simple way to measure building airtightness without the need to have a computer to analyze the Blower Door test data (although a computer program like TECTITE can still be useful to generate reports and store data).

The *Multi-Point Test* procedure involves testing the building over a range of pressures (typically 60 Pascals down to 15 Pascals) and analyzing the data using a Blower Door test analysis computer program (e.g. TECTITE). When conducting a *Multi-Point Test*, we generally recommend that the building be tested at 8 different target pressures between 60 Pa and 15 Pa. For example, a common set of target building pressures includes 60 Pa, 50 Pa, 40 Pa, 35 Pa, 30 Pa, 25 Pa, 20 Pa and 15 Pa. Other target pressures may be used as long as they cover a variety of building pressures between 60 Pa and 15 Pa. Making multiple measurements allows some of the errors introduced by fluctuating pressures and operator error to be averaged out over several measurements, thus increasing test accuracy. In addition, a *Multi-Point Test* allows the operator to estimate the leakage area of the building (i.e. estimate the cumulative size of the hole in the building envelope). Leakage area values are used in detailed infiltration models and can be a useful way to express the results of the Blower Door test.

### 5.2 Depressurization Test Procedures Using the DG-700

The following test procedures cover use of the DG-700 for both *One-Point Tests* and *Multi-Point Tests*.

#### a) Turn on the DG-700 and place it in the proper Mode:

- *DG-700: One-Point Test*

Turn on the gauge by pressing the **ON/OFF** button. Press the **MODE** button twice to put the gauge into the **PR/ FL @50** mode. In this specialized test mode **Channel A** is used to measure building pressure while **Channel B** is used to display estimated building leakage at a test pressure of 50 Pascals (CFM50). The leakage estimate shown on **Channel B** is determined by mathematically adjusting the actual air flow from the Blower Door fan to a test pressure of 50 Pascals, using the real-time **Channel A** building pressure reading and a Can't Reach Fifty (CRF) factor. CRF factors are discussed later in this Chapter.

- *DG-700: Multi-Point Test*

Turn on the gauge by pressing the **ON/OFF** button. Press the **MODE** button once to put the gauge into the **PR/ FL** mode. The **PR/ FL** mode is a multi-purpose mode used to measure a test pressure on **Channel A** while simultaneously measuring air flow from the Blower Door fan on **Channel B**.

**b) Measure the baseline building pressure (same for both *One-Point* and *Multi-Point Tests*).**

When conducting a Blower Door test, we want to measure the change in building pressure caused by air flowing through the Blower Door fan. In order to measure this change accurately, we need to account for any existing pressures on the building caused by stack, wind and other driving forces. This existing building pressure is called the "baseline building pressure".

The DG-700 has a built-in baseline measurement procedure which allows the user to quickly measure and record the baseline pressure on **Channel A**, and then display the baseline adjusted pressure. This feature makes it possible to "zero out" the baseline building pressure on **Channel A**, and display the actual change in building pressure caused by the Blower Door fan.

With the fan sealed off, begin a baseline building pressure reading from **Channel A** by pressing the **BASELINE** button. The word "BASELINE" will begin to flash in the **Channel A** display indicating that the baseline feature has been initiated. Press **START** to start the baseline measurement. During a baseline measurement, **Channel A** will display a long-term average baseline pressure reading while **Channel B** is used as a timer in seconds to show the elapsed measurement time. When you are satisfied with the baseline measurement, press the **ENTER** button to accept and enter the baseline reading into the gauge. The **Channel A** display will now show an **ADJ** icon to indicate that it is displaying a baseline adjusted building pressure value. **Note:** Once a baseline measurement has been taken and entered into the gauge (i.e. ADJ appears below the **Channel A** reading), a new baseline measurement procedure can be initiated by pressing the **BASELINE** button.

**c) Choose a Flow Ring for the Blower Door fan (same for both *One-Point* and *Multi-Point Tests*).**

Remove the No-Flow Plate from the Blower Door fan and install the Flow Ring which you think best matches the needed fan flow. Installation of Flow Rings will depend on the tightness level of the building stock being tested. For example, for relatively leaky buildings (greater than 3,000 CFM50), you will want to start the test using the Open Fan configuration (i.e.

Fan Configuration	Flow Range (cfm) for Model 3 Fan
Open (no Flow Ring)	6,300 - 2,425
Ring A	2,800 - 915
Ring B	1,100 - 300
Ring C	330 - 85

no Flow Rings installed). As you test tighter buildings, you will need to install Flow Rings A or B. Refer to the Table to the right for approximate flow ranges of the fan using the various Flow Rings configurations. Don't worry if you guess wrong and start the test with the incorrect Flow Ring - you can change the Fan Configuration during the test procedure.

**d) Enter the selected Flow Ring into the Gauge (same for both *One-Point* and *Multi-Point Tests*).**

In order for the DG-700 to properly display fan flow, you need to input the Blower Door fan model and selected Flow Ring into the gauge. Check (and adjust if necessary) the selected test Device (i.e. fan) and Configuration (i.e. Flow Ring) shown in the upper part of the gauge display to match the fan and Flow Ring used in the test.

Press the **DEVICE** button to change the selected Blower Door fan.

**Device Icon**

<b>BD 3</b>	Model 3 110V fan
<b>BD 3 220</b>	Model 3 220V fan
<b>BD 4</b>	Model 4 220V fan

Once the fan is selected, the configuration of the fan can be selected by pressing the **CONFIG** button. The currently selected Flow Ring configuration is shown in the Config section of the gauge display.

**Config Icon**

<b>OPEN</b>	No Flow Ring
<b>A1</b>	Ring A
<b>B2</b>	Ring B

**Config Icon**

<b>C3</b>	Ring C
<b>D</b>	Ring D
<b>E</b>	Ring E

Also be sure that **Channel B** is showing the proper air flow units for your test (this should typically be set to **CFM**). Units can be changed by pressing the **UNITS** button.

**e) Turn on the fan for an initial inspection (same for both *One-Point* and *Multi-Point Tests*).**

Turn on the Blower Door fan by slowly turning the fan controller clockwise. As the fan speed increases, the building depressurization displayed on **Channel A** should also increase. As you increase the fan speed, you will be increasing the pressure difference between the building and outside resulting in increased pressure exerted on the aluminum door frame installed in the door opening. If you did not properly install the door frame, the frame may pop out of the doorway at higher building pressures (over 30 Pascals). If this happens, simply reinstall the frame more securely. When installed properly, the frame will easily stay in place during the entire test procedure. Before making measurements, you may want to quickly walk around the building with the fan producing about 30 Pascals of building pressure to check for any problems such as windows or doors blown open or blowing ashes from a fire place or wood stove.

**f) Make final adjustments to the Blower Door fan:**

- *DG-700: One-Point Test*

***If Manually Controlling the Fan:***

Continue to increase fan speed until the building depressurization shown on **Channel A** is between -45 and -55 Pascals. Do not waste time adjusting and re-adjusting the fan speed control to achieve a test pressure of exactly -50 Pascals – just get close to the target pressure. As long you are using the **PR/ FL @50** mode and the test pressure displayed on **Channel A** is within 5 Pascals of the -50 Pascal target pressure, any errors introduced by estimating the leakage on **Channel B** will typically be very small (less than 1%).

***If Using Cruise Control:***

Turn the Blower Door speed control knob to the “just on” position (i.e. the controller is on but the Blower Door fan is not turning). Now press the **Begin Cruise (Enter)** button. The **Channel A** display will now show the number 50 (your target Cruise pressure). Press the **Start Fan (Start)** button. The Blower Door fan will now slowly increase speed until the building depressurization displayed on **Channel A** is approximately 50 Pascals.

**Channel B** will now display the *One-Point* CFM50 leakage estimate. If the leakage estimate is fluctuating more than desired, try changing the Time Averaging setting on the gauge by pressing the **TIME AVG** button and choosing the **5** or **10** second or *Long-term* averaging period. Record the CFM50 test reading on a Test Form (see Appendix D).

Turn off the fan. If you are using Cruise Control, this is done by pressing the **Stop Fan (Clear)** button.

(If “-----” or “LO” appear on **Channel B**, see below).

Whenever “-----” or “LO” appears on **Channel B** in the **PR/ FL @ 50** mode, the DG-700 can not calculate a reliable leakage estimate. The messages “-----” and “LO” appear on **Channel B** under the following three conditions:

- “-----” is continuously displayed when the building test pressure from **Channel A** is below a minimum value of 10 Pascals. Estimating leakage results when the test pressure is below this value may result in unacceptably large errors. If possible, install a larger Flow Ring or remove the Flow Rings to generate more fan flow.
- “LO” is continuously displayed when there is negligible air flow through the test device.

- “LO” alternates with a flow reading when the air flow reading through the device is unreliable (i.e. you are trying to measure a flow outside of the calibrated range of the test device in its current configuration). If possible, you should change the test device configuration to match the flow rate being measured (e.g. install a Flow Ring or a smaller Flow Ring).

**Note:** If you change the Flow Ring on the fan, be sure to change the Configuration setting on the gauge (using the **CONFIG** button) to match the installed Ring. If you are using the Cruise Control feature, you will need to exit Cruise (by pressing the **CLEAR** button) before using the **CONFIG** button to change the selected Flow Ring.

- *DG-700: Multi-Point Test*

Manually increase the fan speed until you achieve the highest target building pressure (e.g. -60 Pascals) on **Channel A**. The fan flow needed to create this building pressure can be read directly from **Channel B**. Record the test readings (building pressure and fan flow) on a Test Form (see Appendix D).

Now reduce the fan speed until the building pressure equals the next target pressure (e.g. -50 Pa). Once again record the test readings on a Test Form. Continue this procedure for each of the remaining target pressures. Turn off the fan when the final set of readings are completed.

Enter the test readings into the TECTITE software to generate your final test results. **Note:** Enter a baseline pressure value of 0 into the TECTITE Manual Data Entry Screen because you “zeroed out” the baseline pressure using the DG-700’s built-in baseline feature.

(If “LO” appears on **Channel B**, see below).

Whenever “LO” appears on **Channel B** in the **PR/ FL** Mode, the DG-700 can not display a reliable fan flow reading. The message “LO” appears on **Channel B** under the following two conditions:

- “LO” is continuously displayed when there is negligible air flow through the test device.
- “LO” alternates with a flow reading when the air flow reading through the device is unreliable (i.e. you are trying to measure a flow outside of the calibrated range of the test device in its current configuration). If possible, you should change the test device configuration to match the flow rate being measured (e.g. install a Flow Ring or a smaller Flow Ring).

**Note:** If you change the Flow Ring on the fan, be sure to change the Configuration setting on the gauge (using the **CONFIG** button) to match the installed Ring.

### **5.3 Depressurization Test Procedures Using the DG-3**

The following test procedures cover use of the DG-3 for both *One-Point Tests* and *Multi-Point Tests*.

**a) Turn on the DG-3 and put it into the proper Mode (same for both *One-Point* and *Multi-Point Tests*).**

Turn the **CHANNEL** knob to **A**, turn the **MODE** switch to **Pressure**, and put the **RANGE** switch in the **Low Range** position (200.0 Pa).

**b) Measure the baseline building pressure (same for both *One-Point* and *Multi-Point Tests*).**

When conducting a Blower Door test, we want to measure the change in building pressure caused by air flowing through the Blower Door fan. In order to measure this change accurately, we need to account for any existing pressures on the building caused by stack, wind and other driving forces. This existing building pressure is called the “baseline building pressure”.

When using the DG-3 gauge, we need to measure and record the actual baseline building pressure (see Appendix D for a sample test recording form). Baseline building pressure is read from **Channel A** of the gauge. With the fan sealed off, record the baseline building pressure on a Test Form, including the sign of the reading (i.e. negative or positive reading). If the pressure is fluctuating too much to determine the reading, try changing the Time Averaging setting on the gauge by turning the **Mode Switch** to **Time Select**, choosing the **5** or **10** second or **Long-term** average, and then return the **Mode Switch** to the **Pressure** setting.

**Note:** If you will be using the TECTITE software, the measured baseline building pressure will need to be entered into the program's Data Table.

**c) Choose a Flow Ring for the Blower Door fan (same for both *One-Point* and *Multi-Point* Tests).**

Remove the No-Flow Plate and install the Flow Ring which you think best matches the needed fan flow. Installation of Flow Rings will depend on the tightness level of the building stock being tested.

For example, for relatively leaky buildings (greater than 3,000 CFM50), you will want to start the test using the Open Fan configuration (i.e. no Flow Rings installed). As you test tighter buildings, you will need to install Flow Rings A or B. Refer to the Table to the right for approximate flow ranges of the fan using the various Flow Rings configurations. Don't worry if you guess wrong and start the test with the incorrect Flow Ring - you can change the Fan Configuration during the test procedure.

Fan Configuration	Flow Range (cfm) for Model 3 Fan
Open (no Flow Ring)	6,300 - 2,430
Ring A	2,800 - 915
Ring B	1,100 - 300
Ring C	330 - 85

**d) Enter the selected Flow Ring into the Gauge (same for both *One-Point* and *Multi-Point* Tests).**

In order for the DG-3 to properly display fan flow, you need to input the Blower Door fan model and selected Flow Ring into the gauge. To select the fan type and fan configuration being used in your test, first turn the **MODE** knob to the **Fan Select** position. The gauge display will show "-SEL" to indicate that a fan type and fan configuration have not yet been selected. The fan type can be selected by toggling the **SELECT** Switch up. The fan configuration can be selected by toggling the **SELECT** switch down.

**If the  
Display  
Shows**

**Description**

- |             |  |
|-------------|--|
| <b>-SEL</b> | Begin fan type selection by toggling the <b>SELECT</b> switch <u>up</u> once.  |
| <b>3-0</b>  | This indicates that you have chosen the Model 3 Minneapolis Blower Door fan, and that the fan is in the "Open" inlet configuration (i.e. no Flow Rings installed).<br><br>To change the fan inlet configuration for the Model 3 Blower Door fan, toggle the <b>SELECT</b> switch <u>down</u> . |
| <b>3-1</b>  | Model 3 Blower Door fan with Ring A installed.   |
| <b>3-2</b>  | Model 3 Blower Door fan with Ring B installed.   |
| <b>3-3</b>  | Model 3 Blower Door fan with Ring C installed.   |
| <b>3-4</b>  | Model 3 Blower Door fan with Ring D installed.   |
| <b>3-5</b>  | Model 3 Blower Door fan with Ring E installed.   |

To change the fan type to the Model 4 Blower Door fan, toggle the **SELECT** switch up twice (DG-3E gauge only).

- |            |  |
|------------|--|
| <b>4-0</b> | This indicates that you have chosen the Model 4 Minneapolis Blower Door fan, and that the fan is in the "Open" inlet configuration (i.e. no Flow Rings installed).<br><br>To change the fan inlet configuration for the Model 4 Blower Door fan, toggle the <b>SELECT</b> switch <u>down</u> . |
|------------|--|

- 4-1 Model 4 Blower Door fan with Ring A installed.
- 4-2 Model 4 Blower Door fan with Ring B installed.
- 4-3 Model 4 Blower Door fan with Ring C installed.
- 4-4 Model 4 Blower Door fan with Ring D installed.
- 4-5 Model 4 Blower Door fan with Ring E installed.

Once you have input the fan configuration, turn the **MODE** knob back to **Pressure**, and then flip the **RANGE** switch to the **2000** setting (**High Range**).

**e) Turn on the fan for an initial inspection (same for both *One-Point* and *Multi-Point* Tests).**

With the **CHANNEL** knob set to **Channel A**, turn on the Blower Door fan by slowly turning the fan controller clockwise. As the fan speed increases, building pressure indicated on **Channel A** should also increase. As you increase the fan speed, you will be increasing the pressure difference between the building and outside resulting in increased pressure exerted on the aluminum door frame installed in the door opening. If you did not properly install the door frame, the frame may pop out of the doorway at higher building pressures (over 30 Pascals). If this happens, simply reinstall the frame more securely. When installed properly, the frame will easily stay in place during the entire test procedure. Before making measurements, you may want to quickly walk around the building with the fan producing about 30 Pascals of building pressure to check for any problems such as windows or doors blown open or blowing ashes from a fire place or wood stove.

**f) Make final adjustments to the Blower Door fan:**

- *DG-3: One-Point Test*

Increase fan speed until the building is depressurized by 50 Pascals from the baseline pressure measured in section **b)** above (i.e. change the building pressure by 50 Pa from the baseline building pressure). In order to do this, you first need to calculate a new adjusted target test pressure to shoot for. This is done by manually adding the measured baseline building pressure to the target depressurization.

***Example:** If the measured building baseline pressure was negative 2 Pascals (-2 Pa), the new target test pressure becomes  $(-2 + (-50))$  or -52. In other words, you will need to depressurize the building to -52 Pascals for your One-Point Test. The main point to remember is that we want to change building pressure by 50 Pascals from the starting point (baseline) pressure.*

***Note:** If you are using the DG-3 and the TECTITE software program, it is not necessary to adjust the target pressure of -50 Pascals for your One-Point Test because the baseline building pressure can simply be entered into the TECTITE Data Table.*

After adjusting the fan speed to depressurize the building by 50 Pascals, turn the **CHANNEL** knob to **Channel B**, and turn the **MODE** switch to **Flow**. The gauge will now display the *One-Point* CFM50 leakage result for the building. If the gauge display is fluctuating too much to determine the reading, try changing the Time Averaging setting on the gauge by turning the **MODE** Switch to **Time Select**, choosing the **5** or **10** second or **Long-term** average, and then returning to the **Flow** mode. Record the CFM50 test reading on a Test Form (see Appendix D). Turn off the fan.

(If the CFM flow reading on **Channel B** is blinking, see below):

- The CFM flow reading on **Channel B** will blink when the air flow reading through the fan is unreliable (i.e. you are trying to measure a flow outside of the calibrated range of the test device in its current configuration). If possible, you should change the fan configuration to match the flow rate being measured (e.g. install a Flow Ring or a smaller Flow Ring).
- If you change Flow Rings, be sure to use the **Fan Select** feature to update the gauge with the new Flow Ring installed before reconducting the test.

- *DG-3: Multi-Point Test*

Increase the fan speed until you achieve the highest target building pressure (e.g. -60 Pascals) on **Channel A**. Now determine the air flow through the fan needed to create this building pressure by first turning the **CHANNEL** switch to **Channel B**, and then turning the **MODE** knob to the **Flow** position. The gauge will now display the flow through the fan. Record the test readings (building pressure and fan flow) on a Test Form (see Appendix D).

Turn the **CHANNEL** switch back to **Channel A** and then turn the **MODE** knob back to the **Pressure** setting. Now reduce the fan speed until the building pressure equals the next target pressure (e.g. -50 Pa). Once again determine the air flow from **Channel B** and record the test readings on a Test Form. Continue this procedure for each of the remaining target pressures. Turn off the fan when the final set of readings are completed.

Enter the test readings into the TECTITE software to generate your final test results.

(If the CFM flow reading on **Channel B** is blinking, see below):

- The CFM flow reading on **Channel B** will blink when the air flow reading through the fan is unreliable (i.e. you are trying to measure a flow outside of the calibrated range of the test device in its current configuration). If possible, you should change the fan configuration to match the flow rate being measured (e.g. install a Flow Ring or a smaller Flow Ring).
- If you change Flow Rings, be sure to use the **Fan Select** feature to update the gauge with the new Flow Ring installed before reconducting the test.

## **5.4 Using the Can't Reach 50 Factors (One-Point Tests)**

If you were performing a *One-Point Test* and the Blower Door fan was unable to depressurize the building by approximately 50 Pascals because one of the Flow Rings was installed, remove the Ring and repeat the test (removing the Flow Ring will increase the maximum air flow available from the fan). If you were not able to depressurize the building by approximately 50 Pascals (with the "Open Fan" running at full speed) because the building is extremely leaky, use the following instructions:

- *For DG-700 Users:*

No adjustments to the test procedure above are necessary other than to make sure the gauge was in the **PR/ FL @50** mode during the *One-Point Test*. If you can not achieve the target test pressure of 50 Pascals because the building is extremely leaky, a CFM50 leakage estimate will automatically be displayed on **Channel B**. The leakage estimate shown on **Channel B** is determined by continuously adjusting the measured air flow from the Blower Door fan to a test pressure of 50 Pascals, using the real-time **Channel A** building pressure reading and the Can't Reach Fifty Factors shown in Table 2 below.

- *For DG-3 Users:*

Take your *One-Point Test* reading at the highest achievable building pressure. Now manually use Table 2 below to estimate the amount of air flow through the Blower Door fan it would take to reach the target pressure. To use Table 2, determine the flow required to maintain the highest achievable building pressure listed in the Table. Multiply this flow by the corresponding "Can't Reach Fifty (CRF) Factor" to estimate flow that would be required to maintain a 50 Pascal building pressure.

Table 2: Can't Reach Fifty Factors

Building Pressure (Pa)	CRF Factor	Building Pressure (Pa)	CRF Factor
48	1.03	28	1.46
46	1.06	26	1.53
44	1.09	24	1.61
42	1.12	22	1.71
40	1.16	20	1.81
38	1.20	18	1.94
36	1.24	16	2.10
34	1.28	14	2.29
32	1.34	12	2.53
30	1.39	10	2.85

*Example:* With the fan running full speed, you are able to achieve a building pressure of 28 Pascals with a measured fan flow of 5,600 cfm. The corresponding CRF Factor for a building pressure of 28 Pascals is 1.46. The estimated flow needed to achieve the target pressure of 50 Pascals is  $5,600 \times 1.46 = 8,176$  cfm.

$$\text{Can't Reach Fifty Factor} = \left\{ \frac{50}{\text{Current Test Pressure (Pa) (Channel A)}} \right\}^{0.65}$$

**Note:** The TECTITE program automatically applies the CRF Factors to *One-Point Test* data.

#### 5.4.a Potential Errors In One-Point CFM50 Estimate from Using the CRF Factors:

Table 3 below show the potential errors in the *One-Point* CFM50 leakage estimates from using the CRF factors. There are two main sources of error:

- The actual test pressure (**Channel A**) not being equal to the target pressure of 50 Pascals.
- The actual exponent of the leaks being measured differing from the assumed exponent of 0.65.

Table 3: Error in *One-Point* Leakage Estimate from CRF factors

		Actual exponent "n"					
		0.5	0.55	0.6	0.65	0.7	0.75
Test Pressure in Pa (Channel A)	10	21.4%	14.9%	7.7%	0.0%	-8.4%	-17.5%
	15	16.5%	11.3%	5.8%	0.0%	-6.2%	-12.8%
	20	12.8%	8.8%	4.5%	0.0%	-4.7%	-9.6%
	25	9.9%	6.7%	3.4%	0.0%	-3.5%	-7.2%
	30	7.4%	5.0%	2.5%	0.0%	-2.6%	-5.2%
	35	5.2%	3.5%	1.8%	0.0%	-1.8%	-3.6%
	40	3.3%	2.2%	1.1%	0.0%	-1.1%	-2.3%
	45	1.6%	1.0%	0.5%	0.0%	-0.5%	-1.1%
	50	0.0%	0.0%	0.0%	0.0%	0.0%	0.0%
	55	-1.4%	-1.0%	-0.5%	0.0%	0.5%	0.9%
	60	-2.8%	-1.8%	-0.9%	0.0%	0.9%	1.8%
	65	-4.0%	-2.7%	-1.3%	0.0%	1.3%	2.6%

For example, Table 3 shows that for a *One-Point* 50 Pa Blower Door building airtightness test, a 2.5% error would be introduced if the leakage estimate was determined at an actual test pressure of 30 Pa (**Channel A**), and the actual exponent of the leaks was 0.60 rather than the assumed value of 0.65.

### **5.5 Unable to Reach a Target Building Pressure During a Multi-Point Test?**

If the Blower Door fan was unable to achieve the highest target building pressure (e.g. 60 Pascals) because one of the Flow Rings was installed, remove the Ring and repeat the test. If you were not able to reach the highest target pressure with the "Open Fan" running at full speed because the building is extremely leaky, take your first set of test readings the highest achievable building pressure. Continue your test by using the remaining target pressures which are less than the highest achievable pressure.

### **5.6 Testing in Windy Weather**

During strong or gusty winds, building pressure readings can vary significantly. As wind gusts contact a building, the actual pressures within the building will change (10 to 20 Pa changes are common in windy weather). Under these conditions, you will need to spend more time watching the gauges to determine the "best" reading. Use of the time-averaging functions can help stabilize readings in windy conditions.

While conducting a multi-point Blower Door test over a wide range of building pressures will tend to even out some of the error introduced from moderate wind fluctuations, significant wind related error can still exist. Under very windy conditions, it is sometimes impossible to manually collect accurate and repeatable test data. Under these conditions, conducting a fully automated test using a DG-700 or APT system may be the only way to collect accurate and repeatable test results. During an automated test hundreds of simultaneous measurements of building pressure and fan flow are quickly collected greatly reducing the variability of tests results due to wind.

### **5.7 Before Leaving the Building**

Be sure you have returned the building to its original condition before leaving. This includes turning the thermostat and water heater temperature controls to their original setting. Always check to see that furnace, water heater and gas fireplace pilot lights have not been blown out during the Blower Door test - re-light them if necessary. Remove any temporary seals from fireplaces, woodstoves or other openings sealed during the test. In addition, combustion safety tests (see Chapter 10) should usually be performed before leaving the house.

## Chapter 6 Basic Test Results

Basic test results from a *One-Point Test* can be manually calculated to provide a quick assessment of the airtightness of the building. For more complicated calculation procedures including analysis of *Multi-Point Test* data, calculated physical leakage areas, estimated natural infiltration rates (including design infiltration rates), estimated cost of air leakage and ventilation guidelines, we recommend that you use the TECTITE program.

### 6.1 Basic Airtightness Test Results

Airtightness test results can be presented in a number of standardized formats.

#### 6.1.a Air Leakage at 50 Pascals:

- *CFM50:*

CFM50 is the airflow (in cubic feet per minute) from the Blower Door fan needed to create a change in building pressure of 50 Pascals (0.2 inches of water column). A 50 Pascal pressure is roughly equivalent to the pressure generated by a 20 mph wind blowing on the building from all directions. CFM50 is the most commonly used measure of building airtightness and gives a quick indication of the total air leakage in the building envelope. When conducting a *One-Point Test* at 50 Pascals of building pressure, you are directly measuring CFM50.

**Note:** *Air Leakage at 50 Pa* can also be presented in units of liters per second (l/s), or cubic meters per second (m<sup>3</sup>/s).

As a point of reference, an old uninsulated two-story Victorian style wood framed house in Minneapolis would likely produce a CFM50 test result in the range of 4,000 to 8,000 - quite leaky. A new modern house built to a strict airtightness standard would likely produce a test result in the 600 to 1,000 CFM50 range - quite airtight - in fact tight enough that a mechanical ventilation system would be needed to maintain good indoor air quality.

The airtightness of existing homes can vary dramatically based on the construction style, age and region. Below are airtightness test results from a few field tests of new and existing homes around the United States.

	Average CFM50
64 New Houses in Minnesota (1984)	1390
22 New Houses in Arizona (1994)	1959
18 New Houses North Carolina (1990)	1987
19 Existing Houses in Arkansas (low-income weatherization)	3071
6,711 Existing Houses in Ohio (low-income weatherization)	4451

- *Percent Reduction in CFM50:*

Performing a *One-Point* CFM50 test before and after airtightening work will allow you to determine the reduction in building airtightness. Reductions in CFM50 as large as 40 to 50 percent are often achieved in high level weatherization programs working on leaky houses. To determine the percent reduction in CFM50, subtract the after-tightening test result from the before-tightening test result. Divide this difference by the before-tightening result and multiply by 100.

$$\% \text{ Reduction} = \frac{\text{CFM50 (before)} - \text{CFM50 (after)}}{\text{CFM50 (before)}} \times 100$$

### 6.1.b Normalizing Air Leakage for the Size of the House:

In order to compare the relative tightness of buildings, it is useful to adjust (or normalize) the results for the size of the building. This allows easy comparison of various size buildings with each other, or with program standards. There are many aspects of building size which can be used to normalize including volume, floor area and surface area of the building envelope.

- *Air Change per Hour at 50 Pascals (ACH50):*

One way to compare different size buildings is to compare the measured *Air Leakage at 50 Pascals* (e.g. CFM50) to the conditioned interior volume of the building. *Air Change per Hour at 50 Pa* or (ACH50) is calculated by multiplying CFM50 by 60 to get air flow per hour, and dividing the result by the volume of the building. ACH50 tells us how many times per hour the entire volume of air in the building is replaced when the building envelope is subjected to a 50 Pascal pressure.

**Note:** If you included the basement of a house in the Blower Door test, (i.e. opened the door between the basement and house during the test) we recommend that you include the basement in your volume calculation.

$$\text{ACH50} = \frac{\text{CFM50} \times 60}{\text{Building Volume (cubic feet)}}$$

Many airtightness test standards for new houses have specified a maximum allowable ACH50 leakage rate. Some examples are listed below.

Example ACH50 Airtightness Standards in New Construction

	ACH50
Canadian R-2000 *	1.5
Alaska Craftsman Home *	1.5
Sweden *	3.0

\* Mechanical Ventilation is required.

The airtightness of existing homes can vary dramatically based on the construction style, age and region. Below are results expressed in ACH50 from a few field tests of new and existing homes around the country.

Measured Field Test Results

	Average ACH50 Pa
64 New Houses in Minnesota (1984)	3.7
129 New Electric Homes in Pacific NW (1987-88)	5.6
134 New Electric Homes in Pacific NW (1980-87)	9.3
98 Existing Homes in Florida	12.7

- *Air Leakage at 50 Pascals per Unit of Floor Area:*

This parameter is calculated by dividing the measured *Air Leakage at 50 Pascals* (e.g. CFM50) by the floor area of the building. Floor area is sometimes used to normalize leakage because floor area is an easily determined number often known by the occupant.

$$\text{CFM50 per Square Foot of Floor Area} = \frac{\text{CFM50}}{\text{Square Feet of Floor Area}}$$

- *Air Leakage at 50 Pascals per Unit of Above Grade Surface Area (Minneapolis Leakage Ratio):*

Also known as the *Minneapolis Leakage Ratio* (MLR), this is the measured *Air Leakage at 50 Pascals* (e.g. CFM50) divided by the above grade surface area of the building. MLR is a useful method of adjusting the leakage rate by the amount of envelope surface through which air leakage can occur. The MLR has been particularly useful for weatherization crews working on wood frame buildings. Experience to date has shown that for uninsulated wood frame houses with a MLR above 1.0, very large cost-effective reductions in house leakage can often be achieved by using dense-pack cellulose insulation techniques and airsealing other large hidden construction openings. In houses with a calculated MLR in the 0.5 to 1.0 range, it is often more difficult to achieve economical improvements in airtightness.

$$\text{Minneapolis Leakage Ratio} = \frac{\text{CFM50}}{\text{Square Feet of Above Grade Surface Area}}$$

**Note:** When calculating Above Grade Surface Area, we recommend including all surfaces separating the conditioned space of the building from unconditioned spaces (e.g. exterior walls, floors over unheated and vented crawlspaces, surfaces separating the building and the attic).

## **6.2 Optional Correction for Air Density**

To increase the accuracy of either a *One-Point Test* or a *Multi-Point Test*, the fan flow measurements can be corrected for differences in air density caused by air temperature. During a depressurization test, the Blower Door system is measuring the air flow through the Blower Door fan. But what we really want to know is the air flow coming back into the building through air leaks. When the inside and outside temperature are different, the air flow leaving the building through the fan is actually different from the air flow back into the building (due to differences in air density). In extreme weather conditions, this difference in air flow can be as great as 10 percent. If you wish to manually adjust your test results for differences in air density, a table of air density correction factors can be found in Appendix H.

**Note:** If you are using the TECTITE program, corrections for air density are made automatically.

### **6.3 Additional Test Result Options (requires use of TECTITE software)**

#### ***6.3.a Leakage Areas:***

Once the leakage rate of the building has been measured, it is often useful to estimate the cumulative size of all leaks or holes in the building's air barrier. The estimated leakage areas provide us with a way to visualize the physical size of the measured holes in the building. In addition, leakage areas are used in infiltration models to estimate the building's natural infiltration rates (i.e. the air change rate under natural weather conditions – see Estimating Natural Infiltration Rates below). In order to accurately estimate leakage areas, it is best to conduct a *Multi-Point* Blower Door test over a range of building pressures (60 Pa to 15 Pa).

Typically, two separate leakage area estimates are calculated based on differing assumptions about the physical shape and behavior of the leaks. These two leakage areas are compatible with the two most commonly used infiltration models.

- **Equivalent Leakage Area (EqLA):** EqLA is defined by Canadian researchers at the Canadian National Research Council as the area of a sharp edged orifice (a sharp round hole cut in a thin plate) that would leak the same amount of air as the building does at a pressure of 10 Pascals. The EqLA is used in the AIM infiltration model (which is used in the HOT2000 simulation program).
- **Effective Leakage Area (ELA):** ELA was developed by Lawrence Berkeley Laboratory (LBL) and is used in their infiltration model. The Effective Leakage Area is defined as the area of a special nozzle shaped hole (similar to the inlet of your Blower Door fan) that would leak the same amount of air as the building does at a pressure of 4 Pascals.

**Note:** The calculated **EqLA** will typically be about 2 times as large as the ELA. When using leakage area calculations to demonstrate physical changes in building airtightness, we recommend using the **EqLA** measurement. Typically, **EqLA** more closely approximates physical changes in building airtightness. For example, if you performed a Blower Door test, and then opened a window to create a 50 square inch hole and repeated the test, the estimated **EqLA** for the building will have increased by approximately 50 square inches from the initial test results.

#### ***6.3.b Estimated Natural Infiltration Rates:***

Estimating the natural infiltration rate of a building is an important step in evaluating indoor air quality and the possible need for mechanical ventilation. Blower Doors do not directly measure the natural infiltration rates of buildings. Rather, they measure the building leakage rate at pressures significantly greater than those normally generated by natural forces (i.e. wind and stack effect). Blower Door measurements are taken at high pressures because these measurements are highly repeatable and are less subject to large variations due to changes in wind speed and direction. In addition, during a Blower Door test all leaks in the building are subjected to approximately the same pressure and they are leaking in the same direction.

In essence, a Blower Door test measures the cumulative hole size, or leakage area, in the building's air barrier (see Leakage Areas above). From this measurement of leakage area, estimates of natural infiltration rates can be made using mathematical infiltration models. The TECTITE software uses the calculation procedure contained in the American Society of Heating Refrigeration and Air Conditioning Engineers (ASHRAE) Standard 136 to estimate the average annual natural infiltration rate for purposes of evaluating indoor air quality and the need for mechanical ventilation.

**Notes on Estimated Annual Infiltration Rates:**

- Daily and seasonal naturally occurring air change rates will vary dramatically from the estimated annual average rate due to changes in weather conditions (i.e. wind and outside temperature).
- The physical location of the holes in the building air barrier compared to the assumptions used in the infiltration model will cause actual annual average infiltration rates to vary from the estimated values. Research done in the Pacific Northwest on a large sample of houses suggests that estimated infiltration rates for an individual house (based on a Blower Door test) may vary by as much as a factor of two when compared to tracer gas tests - one of the most accurate methods of measuring actual infiltration rates.
- The annual average infiltration estimates from ASHRAE Standard 136 should be used only for evaluating detached single-family dwellings, and are not appropriate for use in estimating peak pollutant levels or energy loss due to infiltration. If any of the building leakage is located in the forced air distribution system, actual air leakage rates may be much greater than the estimates provided here. Duct leaks result in much greater air leakage because they are subjected to much higher pressures than typical building leaks. The ASHRAE 136 standard assumes that 1/4 of the building leakage is in the ceiling, 1/4 is in the floor, 1/2 is in the walls, and that leaks are uniformly distributed.

**6.3.c Mechanical Ventilation Guideline:**

It is possible, even easy in the case of new construction or when air sealing work is done by trained, skilled contractors, to increase the airtightness of a house to the point where natural air change rates (from air leakage) may not provide adequate ventilation rates to maintain acceptable indoor air quality. To help evaluate the need for mechanical ventilation in buildings, national ventilation guidelines have been established by ASHRAE. The recommended whole building mechanical ventilation rate presented in this version of TECTITE is based on ASHRAE Standard 62.2-10, and is only appropriate for low-rise residential structures.

**Recommended Whole Building Mechanical Ventilation Rate:** This value is the recommended whole building ventilation rate to be supplied on a continuous basis using a mechanical ventilation system. The recommended mechanical ventilation rate is based on 7.5 CFM per person (or number of bedrooms plus one – whichever is greater), plus 1 CFM per 100 square feet of floor area. This guideline assumes that in addition to the mechanical ventilation, natural infiltration is providing 2 CFM per 100 square feet of floor area..

For buildings where the estimated annual natural infiltration rate (based on the Blower Door test) is greater than 2 CFM per 100 square feet of floor area, the recommended mechanical ventilation rate is reduced to provide ventilation credit for excess infiltration. In these cases, the recommended mechanical ventilation rate is reduced by the following amount:

$$0.5 \times (\text{estimated annual natural infiltration rate (CFM)} - 0.02 \text{ CFM} \times \text{sq. ft. of floor area})$$

**Notes on Ventilation Guidelines:**

- ASHRAE Standard 62.2-10 also contains requirements for local kitchen and bathroom mechanical exhaust systems. These local exhaust systems may be incorporated into a whole building ventilation strategy. Consult Standard 62.2-10 for more information on ventilation strategies and specific requirements and exceptions contained in the Standard.

- Compliance with the ventilation guideline does not guarantee that a moisture or indoor air quality (IAQ) problem will not develop. Many factors contribute to indoor air quality including ventilation rates, sources and locations of pollutants, and occupant behavior. Additional testing (including combustion safety testing) is needed to fully evaluate air quality in buildings. In many cases, a combination of pollutant source control and mechanical ventilation will be required in order to ensure adequate indoor air quality.

### 6.3.d Estimated Cost of Air Leakage:

The TECTITE program estimates the annual cost associated with measured air leakage, both for heating and cooling. The equations used to calculate the annual cost for air leakage are:

$$\text{Annual Heating Cost} = \frac{26 \times \text{HDD} \times \text{Fuel Price} \times \text{CFM50}}{N \times \text{Seasonal Efficiency}} \times 0.6$$

- HDD is the annual base 65 F heating degree days for the building location.
- The Fuel Price is the cost of fuel in dollars per Btu.
- N is the Energy Climate Factor from the Climate Information Screen (adjusted for wind shielding and building height). See Appendix E for more information.
- Seasonal Efficiency is the AFUE rating of the heating system.

$$\text{Annual Cooling Cost} = \frac{.026 \times \text{CDD} \times \text{Fuel Price} \times \text{CFM50}}{N \times \text{SEER}}$$

- CDD is the base 70 F cooling degree days for the building location.
- The Fuel Price is the cost of electricity in dollars per kwh.
- N is the Energy Climate Factor from the Climate Screen (adjusted for wind shielding and building height). See Appendix E for more information.
- SEER is the SEER rating for the air conditioner.

**Note:** Cooling Cost procedure is based on sensible loads only. In hot humid climates, latent loads due to air leakage can be greater than the sensible loads which are estimated by this procedure.

## Chapter 7 Pressurization Testing

Blower Door airtightness measurements are typically performed with the building depressurized relative to the outdoors (i.e. the Blower Door fan exhausting air out of the building). However, under certain conditions it is necessary to conduct a Blower Door test by pressurizing the building. For example, if a Blower Door test is being conducted where there is a fire in a fireplace or woodstove, pressurization testing should be performed to prevent smoke from being drawn into the building through the fireplace. Pressurization testing may also be used to avoid the possibility of pulling known pollutants into the building during the test procedure (e.g. mold from walls or crawlspaces). In addition, some testing procedures (ASTM E779, EN 13829) recommend that both depressurization and pressurization tests be performed, and then averaged to determine building airtightness.


### 7.1 Gauge Set-Up For Pressurization Measurements

Gauges should be set-up inside the building using the following procedures.

#### 7.1.a DG-700 and DG-3 Gauges:

Connect one end of the **Red** tubing to the Channel B Input tap.

The remaining end of the **Red** tubing should be connected to the pressure tap located on the left side of the Blower Door fan electrical box.

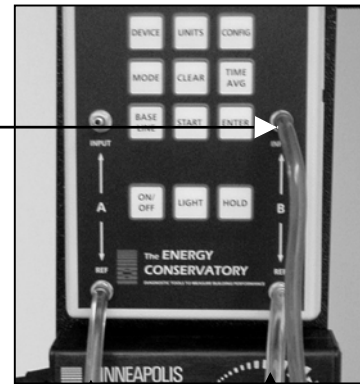

Connect the **Green** tubing to the Channel A Reference tap.


The remaining end of the **Green** tubing should be run to the outside (see Chapter 3 instructions for installing the Outside Building Pressure Tubing).



Connect one end of the extra 30 foot **Clear** tubing (stored in the accessory case) to the Channel B Reference tap.

The remaining end of the **Clear** tubing should be run to the outside, through the open patch at the bottom of the nylon panel. The end of this tubing should be placed next to the side of the fan, but not in the fan's airstream. \*

\* **Note:** Newer Model 4 fans have 2 pressure taps located on the fan electrical box. If your Model 4 fan has 2 pressure taps, connect the remaining end of the **Clear** tubing to the second pressure tap (located by the receptacle), rather than running it to the outside.

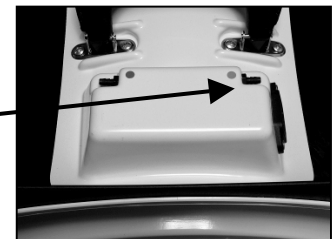


**7.1.b APT System:**

Connect one end of the **Red** tubing to the Channel P2 Input tap.

The remaining end of the **Red** tubing should be connected to the pressure tap located on the left side of the Blower Door fan electrical box.



APT 2

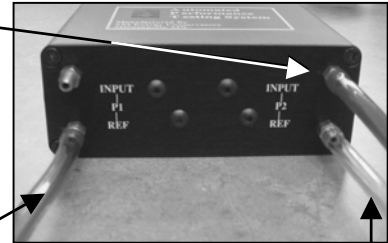

Connect the **Green** tubing to the Channel P1 Reference tap.

The remaining end of the **Green** tubing should be run to the outside (see Chapter 3 instructions for installing the Outside Building Pressure Tubing).




Connect one end of the extra 30 foot **Clear** tubing (stored in the accessory case) to the Channel P2 Reference tap.


The remaining end of the **Clear** tubing should be run to the outside, through the open patch at the bottom of the nylon panel. The end of this tubing should be placed next to the side of the fan, but not in the fan's airstream. \*

Connect one end of the **Red** tubing to the Channel P2 Input tap.

The remaining end of the **Red** tubing should be connected to the pressure tap located on the left side of the Blower Door fan electrical box.



APT 3-8

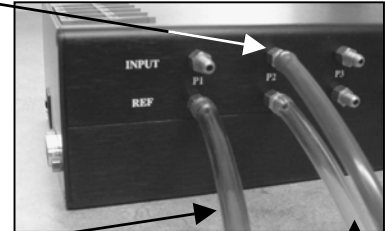

Connect the **Green** tubing to the Channel P1 Reference tap.


The remaining end of the **Green** tubing should be run to the outside (see Chapter 3 instructions for installing the Outside Building Pressure Tubing).



Connect one end of the extra 30 foot **Clear** tubing (stored in the accessory case) to the Channel P2 Reference tap.

The remaining end of the **Clear** tubing should be run to the outside, through the open patch at the bottom of the nylon panel. The end of this tubing should be placed next to the side of the fan, but not in the fan's airstream. \*

\* **Note:** Newer Model 4 fans have 2 pressure taps located on the fan electrical box. If your Model 4 fan has 2 pressure taps, connect the remaining end of the **Clear** tubing to the second pressure tap (located by the receptacle), rather than running it to the outside.

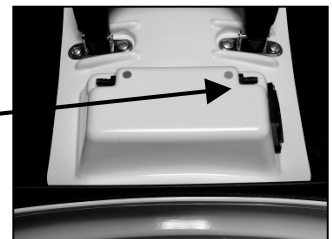

## 7.2 Fan Set-Up For Pressurization Measurements

When pressurizing the building, the fan should be installed with the inlet side of the fan facing outside, and the exhaust side of the fan inside the building. **If you have an older Model 3 fan with a reversible direction switch, be sure to keep the direction switch in the same position as when you perform depressurization tests - we want to blow air into the building through the exhaust guard.** The elastic panel collar should fit snugly around the fan with the collar resting in the gap between the two sides of the electrical box.

The fan is held in place and stabilized by the Velcro strap attached to aluminum frame cross bar. Slip the Velcro strap through the fan handle and loop it up and back around the cross bar. Pull the strap tight so that it is holding the bottom of the fan flange off the floor (approximately 2 inches off the floor if possible.)



You are now ready to make your pressurization measurements using the same testing procedures described in Chapter 5.

## 7.3 Optional Correction for Air Density

Similar to depressurization testing, pressurization fan flow measurements can be adjusted for differences in air density between inside and outside the building. A table of air density correction factors for pressurization testing can be found in Appendix H.

**Note:** If you are using the TECTITE software, corrections for air density are made automatically

## Chapter 8 Finding Air Leaks

There are many techniques that are used to find air leaks with the Blower Door. Air leaks between the interior and exterior of the building often follow long and complicated leakage paths. Typically, the air sealing goal is to find where the leaks cross the "exterior envelope" of the building and to concentrate sealing activities on those areas.

### 8.1 Using Your Hand

The easiest method and one that is used most often is to depressurize the building and walk around the inside, checking for leaks with your hand. When you are looking for leaks, let the Blower Door fan run at a speed which generates between 20 and 30 Pascals of building pressure. You should get in the habit of always using the same pressure so you will get a good feel for what is a big leak and what is not. An entire room can be checked quickly if there is a door between it and the rest of the house. Standing just outside of the room, close the door most of the way, leaving about a one inch crack. A large blast of air coming through this crack indicates large leaks between that room and the outdoors.

### 8.2 Using a Chemical Smoke Puffer

In houses, many of the most important leaks are found between the house and the attic or between the house and a ventilated crawlspace. These leaks usually will not be easy to find unless you physically go into the attic or crawlspace. The use of a handheld smoke puffer is often helpful in these areas. With the house depressurized (and the crawlspace or attic access door shut), you can squirt small puffs of smoke toward suspected leakage sites from the attic or crawlspace and watch to see if the smoke gets sucked into the leak. With a piece of



tubing attached to the smoke puffer, you can often reach deep into corners or in hard to reach spots. A smoke puffer or a pressure pan is a necessity when looking for leaks in the forced air ductwork (see Chapter 9 on duct leakage testing).




**Note:** Smoke from the chemical puffer is very corrosive. Do not store the puffer in a closed container with other items, especially tools or gauges.

### 8.3 Using an Infrared Camera

The ideal technique for finding leaks is to use an infrared scanner with a Blower Door. This procedure usually involves performing two infrared scans from the interior of the building; one before turning on the Blower Door and one after the Blower Door has been depressurizing the building for 5 to 10 minutes. As long as the air being sucked in through the leaks is either warmer or colder than the interior of the house, the area surrounding the leakage path will change temperature and show up on the infrared scanner screen. Even if there is little temperature difference between inside and outside, an infrared scan may still be possible if the attic space has been warmed from solar radiation on the roof or the crawlspace has been cooled from the ground. A temperature difference of about 5 to 10 degrees is sufficient to expose the important leaks. This technique often allows you to find significant leaks without having to enter the attic or crawlspace.

**Note:** Pressurizing the building and inspecting from the outside can also be useful.

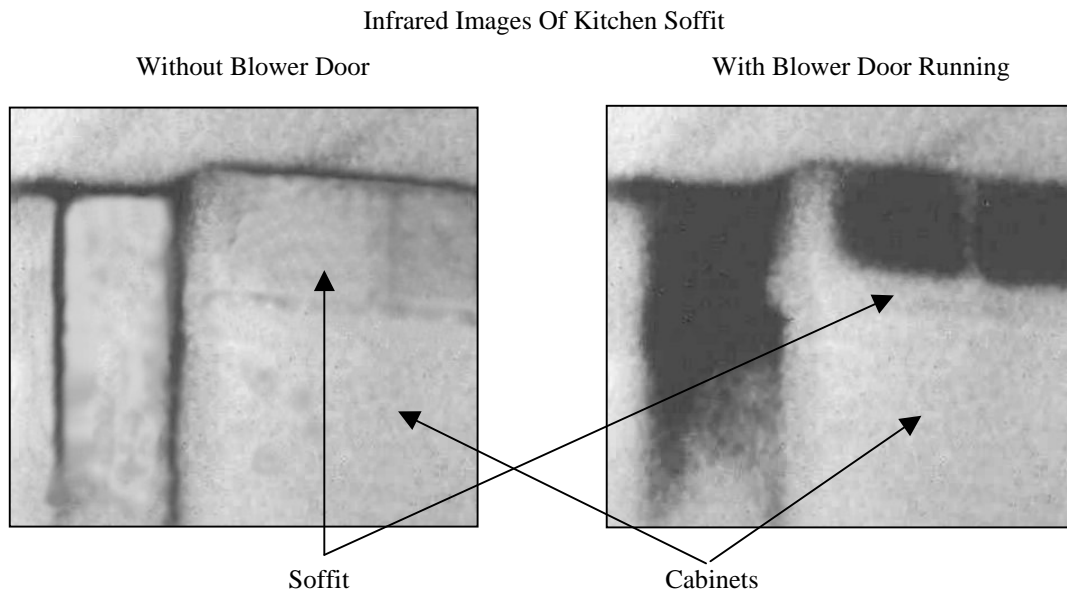

## 8.4 Diagnosing Series Leakage Paths

Many important air leaks in a building are not direct leaks to the outside. Air leaks often follow complicated paths through building cavities and through unconditioned “zones” (such as attics, crawlspaces or garages) on their way into or out of the building. Attic bypasses, found in many houses, are a good example of a series leak. Air leaving the house first must flow through the ceiling/attic boundary and then through the attic/roof boundary before exiting the house.

Diagnostic procedures have been developed over the past decade to analyze series leakage. These procedures, called zone pressure diagnostics (ZPD), are widely used by weatherization professionals to prioritize airsealing efforts in houses by estimating the amount of air leakage from attached zones (e.g. attics, crawlspaces, garages and basements). ZPD techniques typically combine Blower Door airtightness test results with zone pressure measurements made both before and after an opening or hole has been added to one surface of the zone being tested.

In 2000, the Energy Center of Wisconsin commissioned a study of ZPD techniques and procedures in order to improve the accuracy and reliability of zone leakage estimates. The results of that study, published in 2002, include numerous improvements to both the methodology used to collect ZPD measurements and the calculation procedures used to estimate the magnitude of air leakage from tested zones.

To assist our customers in using ZPD calculation methods, we have developed a simple software program which can be used to quickly perform ZPD calculations using many of the improvements recommended in the Energy Center’s study. The ZPD Calculation Utility is comprised of 7 Steps (or screens) which are used to input test information and display test results. The ZPD Calculation Utility program and operation manual are available at no cost from our website ([www.energyconservatory.com](http://www.energyconservatory.com)). The ZPD Calculation Utility assumes that the Blower Door test results and zone pressure measurements are being collected using either an Energy Conservatory digital pressure gauge, or as part of an automated Blower Door test using an APT system.

## **Chapter 9     Testing for Duct Leakage and Pressure Imbalances**

### **9.1 Duct Leakage Basics**

#### ***9.1.a Why Is Duct Leakage Important?***

Unintentional air leakage in forced air duct systems is now recognized as a major source of energy waste in both new and existing houses. Studies indicate that duct leakage can account for 25% or more of total house energy loss, and in many cases has a greater impact on energy use than air infiltration through the building shell. In many light commercial buildings, duct leakage is the single largest cause of performance and comfort problems.

Here are just a few of the problems resulting from duct leakage:

- Leaks in the supply ductwork cause expensive conditioned air to be dumped directly outside or into the attic or crawlspace rather than delivered to the building.
- Leaks in the return ductwork pull unconditioned air directly into the HVAC system reducing both efficiency and capacity. For example, if 10 percent of the return air for an air conditioning system is pulled from a hot attic (120 F), system efficiency and capacity could be reduced by as much as 30 percent. In humid climates, moist air being drawn into return leaks can overwhelm the dehumidification capacity of air conditioning systems causing buildings to feel clammy even when the air conditioner is running.
- Duct leakage has been found to greatly increase the use of electric strip heaters in heat pumps during the heating season.
- Infiltration rates can increase by 2 or 3 times whenever the air handler is operating.
- Leaks in return ductwork draw air into the building from crawlspaces, garages and attics bringing with it dust, mold spores, insulation fibers and other contaminants.
- Building depressurization from duct leaks and imbalanced duct systems can cause spillage of combustion products (from furnaces, water heaters and fireplaces).

#### ***9.1.b Where Does Duct Leakage Occur?***


Because the air leaking from ductwork is invisible, most duct leaks go unnoticed by homeowners and HVAC contractors. In addition, ducts are often installed in difficult to reach spots like attics and crawlspaces, or are "buried" inside building cavities making them even more difficult to find. And the hard to find leaks are usually the most important leaks to fix, because they are connected directly to the outside or to a hot attic or humid crawlspace.

Duct leaks can be caused by a variety of installation and equipment failures including:

- Poorly fitting joints and seams in the ductwork.
- Disconnected or partially disconnected boot connections.
- Holes in duct runs.
- Use of improperly sealed building cavities for supply or return ducts.
- "Platform" return plenums which are connected to unsealed building cavities.
- Poor connections between room registers and register boots.
- Poorly fitting air handler doors, filter doors and air handler cabinets.
- Failed taped joints.

The impact on a particular building will depend on the size of the duct leak, the location of the duct leak and whether or not the leak is connected to the outside.

### Example Duct Leakage Problems

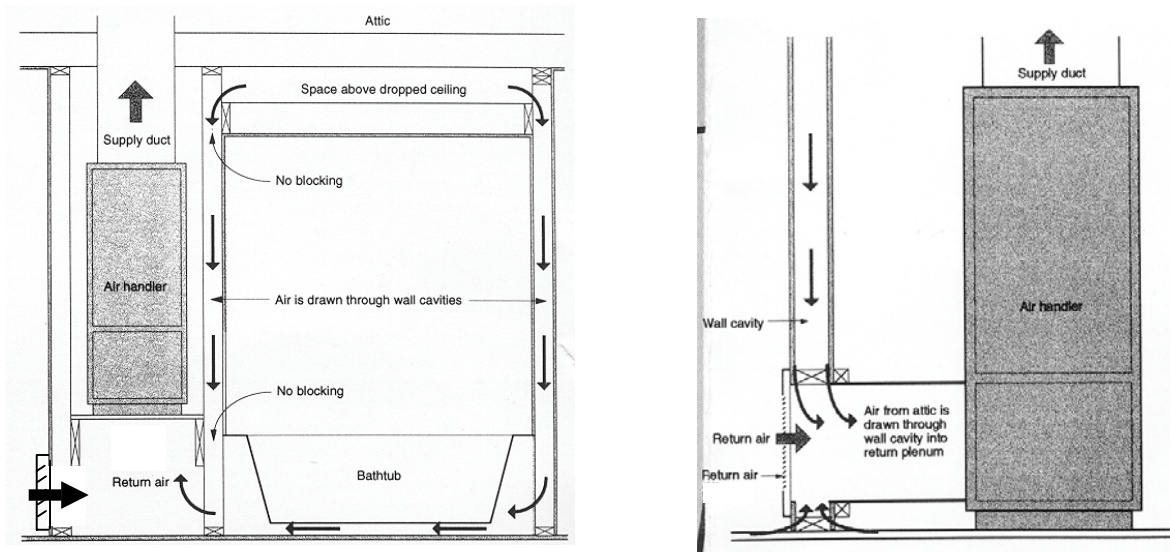

#### 9.1.c How Much Can Energy Bills Be Reduced By Sealing Duct Leaks?

Numerous studies conducted by nationally recognized research organizations has shown that testing and sealing leaky distribution systems is one of the most cost-effective energy improvements available in many houses.

##### A 1991 study in Florida found:

- Air conditioner use was decreased by an average of 17.2% in a sample of 46 houses where comprehensive duct leakage diagnostics and sealing were performed.
- These houses saved an average of \$110 per year on cooling bills at a cost of approximately \$200 for repairs.

##### A 1991 study in Arkansas found:

- Duct leaks also waste energy in heating climates. A study of 18 houses showed that a duct leakage repair service saved 21.8% on heating bills by eliminating three-quarters of the duct leakage in the study houses.

In addition to the energy savings, duct leakage repair improved homeowner comfort and reduced callbacks by allowing the HVAC system to work as designed.

#### 9.1.d Duct Leakage to the Outside:

Duct leakage to the outside has the largest impact on HVAC system performance. Duct leakage to the outside commonly results from leaky ductwork running through unconditioned zones (attics, crawlspaces or garages). Most of the duct leakage research studies referenced in this manual have been performed on houses which contain significant portions of the duct system in unconditioned zones. However, significant leakage to the outside can also occur when all ductwork is located within the building envelope. In these cases, leaky ducts passing through wall or floor cavities (or the cavities themselves may be used as supply or return ducts) create a pressure differential between the cavity containing the ductwork and other building cavities indirectly connected to the outside. Air can be forced through these leaks whenever the air handler fan is operating.

### 9.1.e Duct Leakage to the Inside:

Much less is known about the energy and system efficiency impacts of duct leakage inside the house. A recent study of new houses in Minnesota has shown that the duct systems are very leaky, but that very little of that leakage was connected directly or indirectly to the outside. One of the primary causes of duct leakage in Minnesota houses was found to be very leaky basement return systems which use panned under floor joists as return ductwork. In addition, many of the joints and connections in the sheet metal supply ductwork were leaky. Because almost all of the duct leakage was occurring within the conditioned space of the house, the energy efficiency penalty from this leakage is thought to be much less significant.

However, the Minnesota study did find that leaky return systems can cause the basement (where the furnace and water heater are located) to depressurize to the point where combustion products from the water heater or furnace would spill into the house. Negative pressures from return leaks can also contribute to increased moisture and radon entry into houses. In addition, many comfort problems were experienced in the summer due to leaks in the supply duct system dumping much of the cool conditioned air into the basement. These problems all suggest that controlling duct leakage to the inside may be just as important as leakage to the outside.

## 9.2 Finding Duct Leaks to the Outside

There are a number of simple ways to help you pinpoint which duct runs contain major leaks to the outside. Two methods are presented below:

### 9.2.a Smoke Test:


Turn off the air handler fan, open all registers, remove all filters and open all interior doors. Turn on the Blower Door and pressurize the building to about 25 Pa With Reference To (WTR) outside. With the Blower Door running, go around to all the supply and return registers in the building and squirt a little chemical smoke near the register. If the smoke is vigorously pulled into the register, it indicates that the register is near a large duct leak to the outside. If the smoke lazily moves past the register, little or no outside leakage is near that location.



### 9.2.b Pressure Pan:

An alternative method for finding duct leaks with the Blower Door can be performed with a gasketed pressure pan and a digital pressure gauge. This method involves placing the pressure pan completely over each register and taking a quick pressure reading while the Blower Door is depressurizing or pressurizing the building by 50 Pascals. A measure of the pressure between a duct run and the room where the duct register is located can often provide a quick and reliable indication of whether significant exterior duct leaks exist in that section of the duct system. The pattern of pressure pan readings often allows for quick identification of major leakage sites. Pressure pan readings can also be used to tell technicians if they have done a good job of air sealing the duct system.

Typical pressure pan readings found in existing buildings with external duct systems are commonly in the 0 - 20 Pa range (with the house depressurized to 50 Pa). However, pressure pan readings up to 50 Pa can be found in cases of catastrophic failure (such as complete disconnects). The higher the pressure pan reading, the more connected (leaking) that part of the duct system is to the outside. Experience to date has shown that in many retrofit applications, pressure pan readings can be brought down to, or below, 1.0 Pa with cost-effective duct sealing techniques.

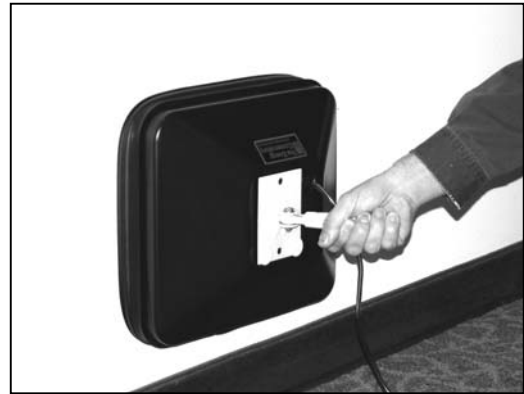

Pressure pan readings do not measure air flow rates. Rather, the pressure pan reading tells us the degree to which a particular duct run is connected to the outside. Because the pressure pan does not measure leakage rates, it is often necessary to make a direct measurement of duct leakage to the outside in CFM to determine if duct repair is cost effective. Further information on pressure pan testing can be obtained from The Energy Conservatory (the Pressure Pan Manual is available on our website at [www.energyconservatory.com](http://www.energyconservatory.com)).

### **9.3 Estimating Duct Leakage to the Outside With a Blower Door**

The following two testing procedures can be used to estimate the amount of leakage directly between the forced air duct system and the outside. **Note:** The leakage rate of a duct system determined using the airtightness test procedures listed in this manual may differ from the leakage rates occurring in the duct system under actual operating conditions. When conducting an airtightness test, all leaks in the ductwork are subjected to approximately the same pressure (i.e. the test pressure). Under actual operating conditions, pressures within the duct system vary considerably with the highest pressure present near the air handler, and the lowest pressures present near the registers. Researchers are working on developing new test procedures which will provide duct leakage measurements under actual operating conditions.

#### ***9.3.a Modified Blower Door Subtraction:***

##### **Step 1: Conduct "Whole House" Blower Door Depressurization Test**

- Set up the building for a standard Blower Door depressurization test.
- Turn the air handler fan off, open all registers and remove all HVAC filters including remote filters.
- Temporarily seal all exterior combustion air intakes and ventilation system air intakes that are connected to the duct system.
- Depressurize the building by 50 Pa With Respect To (WRT) outside (see Chapter 5).
- Record ***Whole House CFM50***, and turn off the Blower Door.

##### **Step 2: Conduct "Envelope Only" Blower Door Depressurization Test**

- Tape off all supply and return registers with Duct Mask temporary register sealing film (available from The Energy Conservatory) or use paper and high quality painters masking tape. Be sure to include any ventilation system supply and return registers that are connected to the forced air duct system.
- Depressurize the building to 50 Pa WRT outside with the Blower Door.
- Record ***Envelope Only CFM50***.

##### **Step 3: Measure Pressure in Duct System with Registers Taped Off**

- With the building still depressurized to 50 Pa WRT outside, measure the pressure in the taped off duct system WRT the building. This measurement can be taken at the return or supply plenum using a static pressure probe, or at a supply or return register by punching a small hole through the sealing tape and inserting a pressure tap or hose.

**Step 4: Calculate Duct Leakage to the Outside**

- Using the pressure measured in Step 3, look up the appropriate correction factor in Table 4 below. This correction is needed to account for any underestimation of duct leakage due to connections between the duct system and the building.
- Calculate Duct Leakage to Outside =

$$(\text{Whole House CFM50} - \text{Envelope Only CFM50}) \times \text{Subtraction Correction Factor (SCF)}$$

Table 4:

### Correction Table For Blower Door Subtraction

House to Duct Pressure (taped off)	Subtraction Correction Factor (SCF)	House to Duct Pressure (taped off)	Subtraction Correction Factor (SCF)
50	1.00	30	2.23
49	1.09	29	2.32
48	1.14	28	2.42
47	1.19	27	2.52
46	1.24	26	2.64
45	1.29	25	2.76
44	1.34	24	2.89
43	1.39	23	3.03
42	1.44	22	3.18
41	1.49	21	3.35
40	1.54	20	3.54
39	1.60	19	3.74
38	1.65	18	3.97
37	1.71	17	4.23
36	1.78	16	4.51
35	1.84	15	4.83
34	1.91	14	5.20
33	1.98	13	5.63
32	2.06	12	6.12
31	2.14	11	6.71

#### *Uncertainty of Duct Leakage Measurements Using Blower Door Subtraction*

Because Blower Door Subtraction involves subtraction of two separate Blower Door test results (using the same Blower Door), the accuracy of the duct leakage estimate using this technique is a function of the repeatability of the Blower Door measurements. The example below shows how repeatability errors can affect the accuracy of Blower Door subtraction test results.

Assume you conducted a Blower Door subtraction test with the following results:

- Whole House CFM50 = 3,000
- Envelope Only CFM50 = 2,750
- House to Duct Pressure During Envelope Only Measurement = 45 Pascals
- Correction Factor = 1.29

The estimated duct leakage would be  $(3,000 - 2,750) \times 1.29 = \underline{322 \text{ cfm}}$

On a day with only slight wind, our experience is that the repeatability of manual Blower Door test is about +/- 3% of the unsealed whole house CFM50 value when using the same gauges for both tests. For the example above, a repeatability error of 3% means we have an error of approximately +/- 90 CFM50 ( $0.03 \times 3,000$  CFM50) in our leakage estimate. We must also apply the correction factor calculated above to the 90 CFM50 error which increases the error to +/- 116 CFM50 ( $90 \times 1.29$ ). Thus our final duct leakage estimate is 322 CFM50 (+/- 116 CFM50). This means the actual leakage in the duct system is somewhere between 206 CFM50 and 438 CFM50, a fairly wide variation in test results.

In very windy weather, repeatability error for a manual Blower Door test will increase to much larger than the 3% shown here. However, if you are using an APT system to conduct your Blower Door test, repeatability errors will typically be reduced below the 3% quoted above, and the APT system will provide you with a estimate of the measurement uncertainty.

### 9.3.b Flow Hood Method: *(Requires use of calibrated flow capture hood)*

- Set up the building for a standard Blower Door pressurization test (see Chapter 7).
- Turn the air handler fan off, open all registers and remove all HVAC filters including remote filters.
- Temporarily seal all exterior combustion air intakes and ventilation system air intakes that are connected to the forced air duct system.
- Tape off all supply and return registers, ***except the largest and closest return to the air handler***, with Duct Mask temporary register sealing film (available from The Energy Conservatory) or use paper and high quality painters masking tape. Include all ventilation system registers connected to the forced air duct system.
- Pressurize the building to 50 Pa WRT outside with the Blower Door.
- Place the flow capture hood over the open return register and record the flow going into the return register. This measured flow is an estimate of the CFM50 duct leakage to the outside.

**Note:** This procedure can also be conducted by depressurizing the building and measuring the air flow coming out of the open return register.

## 9.4 Unconditioned Spaces Containing Ductwork

When using either duct leakage measurement method described in Section 9.3 above, the unconditioned spaces containing ducts should be as close to outside pressure as possible. Be sure to open all operable vents between the unconditioned space and the outside before conducting the duct leakage test. If the unconditioned space containing ductwork is not well connected to the outside (e.g. unvented crawlspaces or unvented attics) or has very large connections to the house, then the unconditioned space will be at a pressure somewhere between the outside and inside building pressure during the Blower Door test. In this case, the duct leakage measurement will show an artificially low number.

You can measure the degree of connection between an unconditioned space and the outside by measuring the pressure difference between the building and the space during the Blower Door test. If the pressure between the building and the unconditioned space is less than 45 Pa (assuming the building to outside pressure difference is 50 Pa with the Blower Door running), then the duct leakage measurement will be underestimated. The lower the pressure, the greater the underestimation.

## **9.5 Testing for Pressure Imbalances Caused By Forced Air System Flows**

Air handler fans commonly move 500 to 2000 cubic feet of air per minute (CFM). Pressure imbalances within the building can be caused by air handler fan operation if supply and return air flows to each part of the building are not in balance. Pressure imbalances within the building can significantly increase infiltration rates, contribute to radon and moisture entry, create durability problems, and cause potential combustion appliance spillage and backdrafting. Research on combustion appliances has found that very small negative pressures (as low as 3 to 5 Pascals) can cause spillage and backdrafting in natural draft appliances.

Building pressure imbalances can also be caused by duct leakage to the outside. If either the supply or return air ductwork has leaks to the outside, air will be forced through these leaks when the air handler fan is operating. If the leaks are in the supply ducts, building air will be exhausted to the outside through the leaks and this will tend to depressurize the building. If the leaks are in the return system, outside air will be sucked into the leaks and the building will tend to be pressurized. If there are equal amounts of leakage in both the supply and return, no change in building pressure will occur, even though large energy losses may result.

Below are a set of test procedures used to help identify pressure imbalances caused by leaks between the duct system and the outside, and by imbalanced supply and return air flows throughout a building. These tests are very sensitive to wind effects, and on windy days it can be very difficult to get accurate results.

### ***9.5.a Dominant Duct Leak Test:***

This test measures whole building pressurization or depressurization caused by duct leakage to the outside during operation of the air handler fan. A pressure change due to duct leakage can cause safety, durability, comfort, and efficiency problems. In some cases, duct repair can cause a problem or make it worse. Diagnosing which side of the system is causing a dominant pressure helps determine a safe and effective treatment strategy.

- Turn off the Blower Door and close off the Blower Door fan opening with the "No-Flow" plate.
- Be sure all exterior doors and windows in the building are closed. Replace all HVAC filters (be sure they are clean). Open all interior doors and check that all exhaust fans and the air handler fan are off.
- Set up a digital gauge to measure the building pressure With Respect To (WRT) outside. The outside pressure hose should be connected to the bottom (Reference) pressure tap on **Channel A** (top tap should be open). Set the gauge Mode to measure pressures.
- Turn on the air handler fan and record the change in building pressure indicated on the gauge.
- Repeat this test several times by turning the air handler on and off for better certainty.
- Greater leakage on the return side of the duct system will typically cause the building to become pressurized since the return ductwork is drawing outside air into the ductwork. In this case, there will be a positive reading on pressure gauge. The size of the pressure change will depend on both the amount of imbalanced duct leakage and the tightness of the building being tested (see Figure 10 in Chapter 10).

- Greater leakage on the supply side of the system will typically cause the building to become depressurized since the supply ductwork is exhausting building air to the outside, just like an exhaust fan. In this case, there will be a negative reading on the pressure gauge. The size of the pressure change will depend on both the amount of imbalanced duct leakage and the tightness of the building being tested (see Figure 10 in Chapter 10).

In cold climates, pressurizing a building to even 1 Pascal could lead to moisture problems caused by forcing warm, moist air into the walls and attic where it can condense on cold surfaces. In warm humid climates, depressurization by 1 Pa can also cause severe moisture problems from warm moist outside air being drawn into the walls where it can condense on the backside of cooled gypsum board. If there are natural draft combustion appliances, or if radon is a problem, depressurizing a building by 1 Pascal may also be a problem.

If there is no change in building pressure, this means that there is either equal supply and return leakage to the outside, no leaks to the outside, or the building itself is too leaky for the duct leakage to create a measurable pressure change.

**Note:** For APT users, a prototype software program called ONOFF is available to help precisely measure small changes in building or room pressures. The program uses a signal averaging technique which significantly reduces noise, particularly in windy weather, allowing for precise measurement of small pressure changes. Contact The Energy Conservatory for more information.

### ***9.5.b Master Suite Door Closure:***

This test measures the effect of closing the master suite door on the pressure in the main body of the building. The master bedroom is often the largest room in a building and can contain multiple supply registers while having no returns. Closing of bedroom doors can restrict the supply air pathway back to the air handler, causing bedrooms to become pressurized while other parts of the building may become depressurized. Repeat this test for other building areas that contain large numbers of registers and can be closed off from the main body of the building with one door (e.g. a basement door when the basement has supply registers).

- Keep the gauge set up to measure the pressure between the main body of the building WRT outside.
- With air handler still running, close the master suite door.
- Record the total pressure difference from the main body of the building WRT outside. (Large impacts from Master Suite Door Closure are most common in single and double return houses.)
- Consider pressure relief if the Master Suite door is frequently closed and causes the pressure in the main body of the building to change by 1 Pascal or more in either direction.

### ***9.5.c All Interior Doors Closed:***

This test measures the added effect of closing all interior doors on the pressure in the main body of the building.

- Keep the gauge set up to measure the pressure between the main body of the building WRT outside.
- With the air handler still running, close all interior doors.
- Record the total pressure difference from the main body of the building WRT outside.
- Consider pressure relief if closing all the doors causes the pressure in the main body of the building to change by 2 Pascals or more in either direction.

### ***9.5.d Room to Room Pressures:***

This test measures the pressure difference between each room in the building and the main body, with the air handler operating. Excessive pressurization in rooms can create durability problems by driving moisture into walls, ceilings and floors. Excessive depressurization in rooms can pull outside moisture into building components in humid climates. Pressure imbalances can also lead to large increases in building infiltration rates.

- Close all interior doors and walk around the building with a digital pressure gauge.
- Connect tubing to the **Channel A** Input tap and leave the bottom Reference tap open. Set the gauge Mode to measure pressures.
- While standing in the main body of the building, place the hose from the gauge under each door (including the combustion appliance room and/or basement).
- Record the pressure difference from each room WRT the main body.
- Consider pressure relief for any rooms pressurized or depressurized by 3 Pa or more with respect to the main body of the building.

**Note:** If there are combustion appliances in a depressurized area (i.e. fireplaces, furnace or water heater), their ability to draft properly may be affected. Try to eliminate all depressurization in combustion appliance zones by finding and sealing leaks in the return ducts, plenum, filter access door and air handler cabinet, or by providing pressure relief. See Chapter 10 for more information on Combustion Safety Testing Procedures.

## **9.6 Other Important Test Procedures**

Although not covered in this manual, other important test procedures should be performed whenever repairs and changes are made to the forced air heating and cooling system.

### ***9.6.a Total System Air Flow:***

The air flow rate through air handlers is a very important variable in estimating and optimizing the performance of heat pumps, air conditioners and furnaces. Many studies of residential systems have shown low air flow to be a common problem. There are a number of methods to measure total system air flow including the Duct Blaster® pressure matching method, the temperature rise method, system static pressure and fan curve, as well as a new direct flow measuring tool (TrueFlow™ Flow Plate) available from TEC.

**Note:** Research has shown that in most cases, the temperature rise method and fan curve method are much less accurate than either the Duct Blaster or TrueFlow methods.

### ***9.6.b System Charge:***

Having the proper amount of refrigerant installed in a new heat pump or air conditioning system is another critical variable in determining system efficiency, as well the longevity of the system compressor. Numerous studies have shown the incorrect amount of system charge to be a common installation problem.

### ***9.6.c Airflow Balancing:***

Verification that proper air flow is being delivered to each room in a building is another important component of a complete system assessment. Air flow rates are commonly measured using a calibrated flow capture hood.

## Chapter 10 Combustion Safety Test Procedure

### 10.1 Overview

Buildings with natural draft combustion appliances should be routinely tested to ensure that the spillage of combustion products into the building is unlikely. Combustion safety testing is critical because of the potential for severe health effects from improperly venting appliances, including carbon monoxide poisoning. Because the goal of Blower Door guided air sealing activities is to reduce the infiltration rate (and subsequent ventilation rate) of the building, contractors need to check that they are not leaving a building with a potential problem.

Spillage of combustion products into the building can be caused by a variety of conditions including:

- Blocked or partially blocked chimneys, vents, or vent connectors.
- Improper equipment installation.
- Cracked heat exchangers.
- Leaks in the venting system (disconnected flue pipes, open cleanout door etc.).
- Low vent temperatures.
- Combustion appliance zone depressurization. As buildings are made tighter, it becomes easier for exhaust fans and forced air system imbalances to create potentially hazardous depressurization conditions.


Many cases of improperly venting combustion appliances have been related to depressurization (or negative pressures) in the room that contains the combustion appliance. Depressurization can be caused by exhaust fans, dryers, imbalanced forced air distribution systems, and forced air system duct leakage. As buildings (or combustion appliance rooms) are made tighter, these problems can be made worse, although very leaky buildings can also have venting problems related to depressurization. Figure 10 below estimates the amount of depressurization that can be caused by various exhaust fan flows. For example, from Figure 10 we can see that a 400 cfm exhaust fan will depressurize a 2,500 CFM50 building (or room) to approximately 3 Pascals. That same 400 cfm fan would produce over 10 Pascals of depressurization in a 1,000 CFM50 building.

The presence of code approved combustion air intakes does not ensure that venting problems will not occur. Significant combustion room depressurization is frequently found even after code approved combustion air intakes have been installed. Passive combustion room air intakes typically do not provide sufficient airflow to relieve negative pressures caused by distribution imbalances, duct leakage, or large exhaust appliances. For example, a typical 6" passive inlet can at best supply only about 50 cfm at a 5 Pa negative building pressure. And because passive air intakes are often poorly installed (i.e. many sharp bends, long runs), they typically provide much lower flows than designed. Building codes typically give little or no guidance on how one would design a combustion air opening when competing exhaust appliances are present (the 2000 Minnesota Energy Code is the only code we are aware of to give such guidance).

The only way to be reasonably sure that venting problems will not occur in a building is to perform combustion safety tests. Described below are commonly used test procedures to locate existing or potential combustion safety problems in buildings. **These procedures are offered only as an example of what other organizations in North America typically recommend for testing. The Energy Conservatory assumes no liability for their use, and contractors should have a working knowledge of local codes and practices before attempting to use the procedures outlined below.**

If combustion safety problems are found, tenants and building owners should be notified immediately and steps taken to correct the problem including notifying a professional heating contractor if basic remedial actions are not available. Remember, the presence of elevated levels of carbon monoxide in ambient building air or in combustion products is a potentially life threatening situation. **Air sealing work should not be undertaken until existing combustion safety problems are resolved, or unless air sealing is itself being used as a remedial action.**

Figure 10:

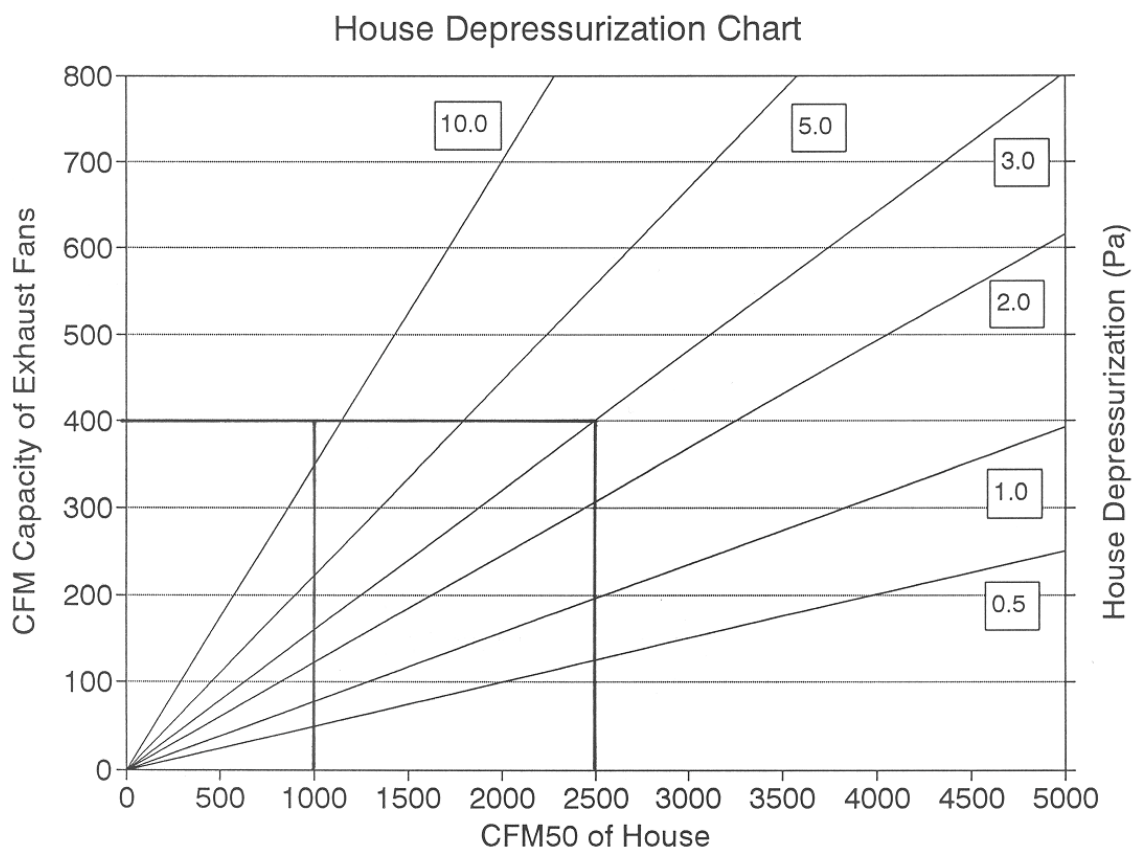

This chart can be used to estimate the amount of house depressurization caused by operating exhaust fans. To use the chart, find the intersection between the airtightness (CFM50) of the house and the cfm capacity of the exhaust fans in question. The amount of depressurization caused by the fan(s) is read off the diagonal house depressurization lines. For example, a 400 cfm kitchen range hood operating in a house with an airtightness level of 2,500 CFM50 would depressurize the house by approximately 3 Pa relative to the outside. This same fan operating in a 1,000 CFM50 house would produce over 10 Pa of depressurization.

Note: This chart was generated by assuming that all houses have a "House Leakage Curve" with an exponent (or slope) of  $n = 0.65$ ,

## **10.2 Test Procedures**

This procedure is not intended to cover all circumstances you will find in the field. A basic understanding of the dynamic interactions between building pressures, air flow and mechanical system operation is required to fully utilize the procedures presented below. Detailed descriptions of similar test procedures can be found in Reference #4, in Appendix G.

**10.2.a Measure Ambient CO Level in Building:**

- Zero your digital CO tester outside before entering the building. CO tester should have 1 PPM resolution.
- Measure the ambient CO level in all occupied areas of the building. Be sure to measure ambient CO levels in kitchens and in combustion appliance rooms.
- Investigate any ambient CO levels above 2 ppm. **Note:** Areas close to very busy streets may have ambient CO levels above 2 ppm.
- Maximum CO concentration guidelines:
 

9 ppm for 8 hour exposure (EPA)
35 ppm for 1 hour exposure (EPA)
200 ppm single exposure (OSHA)

**CO concentrations at or above these levels requires immediate remedial action.**

**10.2.b Survey of Combustion Appliances:**

- Walk through the building and survey all combustion appliances including furnaces, water heaters, fireplaces, woodstove and auxiliary heating units, dryers and cooking stoves.
- Write down the following information on a survey form:
  - Location, type and input of combustion appliances.
  - Signs of visible deterioration and leaks in flue pipes and connections.
  - Presence of gas leaks, signs of spillage or flame roll-out.
  - Location, size and operable condition of combustion air supply(s).
  - Evidence of rusted interior surfaces of heat exchangers.

**Gas or fuel leaks are a very serious safety problem requiring immediate remedial action.**

**10.2.c Survey of Exhaust Fans:**

- Walk through building and note the location and rated capacity (or estimated capacity) of all exhaust fans including kitchen and stove fans, bath fans, dryers, whole house vacuum systems, attic (not whole house) vent fans etc..

**10.2.d Measure Worst Case Fan Depressurization:**

With this test procedure, the goal is to measure worst case depressurization in all combustion rooms with natural draft appliances and fireplaces. This measurement gives us an indication of the likelihood of exhaust and air handler fans causing the combustion appliances to backdraft and spill. The procedures below measure worst case depressurization under 3 separate operating conditions; running exhaust fans only, running exhaust and air handler fans, and running the air handler fan only. These tests are very sensitive to wind effects, and on windy days it can be very difficult to get accurate results.

**Initial Preparation**

Close all exterior windows and doors and be sure furnace, water heater and other vented combustion appliances are off. Close all interior doors. Set up a digital gauge to measure the pressure difference of the combustion appliance zone (CAZ) with reference to (WRT) outside on **Channel A**. If using a DG-3 gauge, record the baseline CAZ to outside pressure. If using a DG-700, use the built-in “baseline” feature to measure and record the baseline CAZ to outside pressure on **Channel A**. Once the “baseline” feature has been used with the DG-700, **Channel A** will display the baseline adjusted pressure.

## 1. Exhaust Fans Only

Turn on all exhaust fans found in the survey above (for dryer, clean out lint filter before turning on). Now determine the worst case position of interior doors with the smoke test below:

**Smoke Test:** While standing in the main body of the building, squirt smoke under each door containing an exhaust fan (except the CAZ currently being tested). If the smoke goes into the room, open the door. If the smoke comes back into the main body of the building, keep the door closed. Now squirt smoke under the CAZ door (while continuing to stand in the main body). If smoke goes into the CAZ, leave the CAZ door shut. If smoke comes back into the main body of the building, open the door.

Measure the depressurization of the CAZ WRT outside caused by turning on the exhaust fans. Depressurization should not exceed the appropriate House Depressurization Limits (HDL) listed below. If it is windy, it is often necessary to turn fans off and on several times to obtain good pressure readings.

**Fireplace Zones:** For Fireplace Zones, repeat the same procedure and measure and record depressurization of fireplace zone WRT outside from exhaust fan operation. Depressurization should not exceed the appropriate HDL listed below.

## 2. Air Handler and Exhaust Fans

With exhaust fans continuing to run, turn on the air handler fan (note: air handler fan only, do not turn on burner) and close any supply registers in combustion appliance room. For both CAZ and Fireplace Zone tests, re-determine worst case position of all interior doors with the smoke test described above. If cooling is available, be sure air handler fan is running at high speed. Repeat worst case depressurization measurements.

## 3. Air Handler Fan Only

Turn off all exhaust fans and leave air handler operating (if cooling is available, be sure air handler is running at high speed). For both CAZ and Fireplace Zone tests, re-determine worst case position of all interior doors with the smoke test described above. Repeat worst case depressurization measurements.

**If the HDL are exceeded for any of the worst case depressurization tests above, pressure relief is needed.** Pressure relief could include duct system repair, undercutting of doors, installation of transfer grills, eliminating or reducing exhaust fan capacity, or instructing homeowner on safe exhaust fan operation. If negative pressures in the combustion appliance zone (or basement) are a function of return leaks in that area, check for leaks in the return ductwork, plenum, filter access door and air handler cabinet. Pay particular attention to panned under floor joists (used as returns) as they typically have many leaks.

**Note:** For APT users, a prototype software program called ONOFF is available to help precisely measure small changes in building or room pressures. The program uses a signal averaging technique which significantly reduces noise, particularly in windy weather, allowing for precise measurement of small pressure changes. Contact The Energy Conservatory for more information.

**Table 5: House Depressurization Limits (HDL)**

Appliance Type	Depressurization Limit
Individual natural draft water heater (WH)	2 Pascals
Natural draft WH <u>and</u> natural draft furnace/boiler	3 Pascals
Natural draft WH <u>and</u> Induced Draft (ID) furnace/boiler	5 Pascals
Individual natural draft furnace/boiler	5 Pascals
Individual ID furnace/boiler	15 Pascals
Power vented and sealed combustion appliances	>25 Pascals

**Source:** CEE Appliance Safety Test Methods, MAC Part 150 Residential Sound Insulation Program, Mpls, MN.

### 10.2.e Spillage Test (natural draft and induced draft appliances):

This test identifies actual spillage of combustion byproducts into the living space under worst case depressurization conditions.

- With building set up in worst case depressurization mode (as specified above), fire up each combustion appliance.
- If appliances are common vented, conduct test on smallest input appliance first, then test with both appliances running.
- When burner lights, check for flame rollout (stand away from burner).
- Check for spillage (using chemical smoke) at the end of the spillage test period (see Table 6 below). For natural draft appliances, spillage is tested at the draft diverter. When an induced draft heating system is vented in common with a natural draft water heater, spillage is checked at the water heater draft diverter. For a single induced draft appliance, spillage is checked at the base of the chimney liner or flue, typically using the drip tee at the bottom of the liner.

**Table 6: Spillage Test Period**

Appliance Type	Spillage Test Period (minutes)
Water heater, gravity furnace and boiler	3.0 minutes
Space heater	2.0 minutes
Furnace	1.0 minutes

**Source:** CEE Appliance Safety Test Methods, MAC Part 150 Residential Sound Insulation Program, Mpls, MN.

- If spillage continues beyond the spillage test period, remove the negative pressure in combustion room by turning off fans and/or opening an exterior window or door.
- Re-check for spillage. If spillage stops, there is a pressure induced spillage problem. If spillage continues, check flue and chimney for obstructions, and check compatibility of appliance BTU input with chimney size.

**Spillage of combustion products beyond the spillage test period is a health and safety concern.** If the problem is a blocked flue or chimney, or inadequately sized flue or chimney, consult a professional heating contractor. If the problem is pressure induced, provide pressure relief. Re-check for spillage following attempt to provide pressure relief. If spillage continues, contact a professional heating contractor to investigate the problem.

**10.2.f Carbon Monoxide Test:**

This test measures carbon monoxide levels in all operating combustion appliances.

- After 5 minutes of appliance operation, measure the CO level in the flue products of all combustion appliances.
- CO should be measured before appliance draft diverter, or barometric damper.
- CO levels should be below 100 ppm in all flues.
- For gas stoves, measure CO from oven exhaust port and 3 feet above burners with all burners running. CO level should be below 50 ppm.
- If CO found in gas stove, re-measure ambient kitchen CO after 10 minutes of stove operation.

**The presence of CO and spillage requires immediate remedial action.**

**10.2.g Draft Test (natural draft appliances):**

This test measures flue draft pressure in the venting systems of all natural draft combustion appliances under worst case depressurization (not to be done for sealed combustion or induced draft appliances).

- Drill a small hole in the vent pipe approx. 2 feet downstream of the draft diverter or barometric damper. Insert a static pressure probe.
- Measure draft pressure (vent WRT combustion room) with digital pressure gauge after 5 minutes of operation.
- Compare measured draft with minimum draft pressures below:

**Table 7: Minimum Draft Pressures**

<b><u>Outside Temp</u></b>	<b><u>Draft Pressure</u></b>
<i>Below 10 F</i>	<i>-2.50 Pa</i>
<i>20 F</i>	<i>-2.25 Pa</i>
<i>40 F</i>	<i>-1.75 Pa</i>
<i>60 F</i>	<i>-1.25 Pa</i>
<i>80 F</i>	<i>-0.75 Pa</i>
<i>Above 90 F</i>	<i>-0.50 Pa</i>

**Source:** CEE Appliance Safety Test Methods, MAC Part 150 Residential Sound Insulation Program, Mpls, MN.

**If measured draft is below the minimum draft pressure above, check for flue or chimney obstructions, disconnected vents, open chimney cleanout doors etc.. Also remove sources depressurization (e.g. turn off exhaust fans) and test again to determine if CAZ depressurization is contributing to poor draft.**

**10.2.h Heat Exchanger Integrity Test (Forced Air Only):**

This test is used to determine if a crack or hole is present in the furnace heat exchanger. A crack or hole could allow products of combustion into the building, and/or promote carbon monoxide production through flame distortion and impingement. There are 3 main types of tests which can be performed:

**1. Flame Distortion Test**

This test involves watching the furnace flame when the furnace air handler first turns on. Any distortion of the flame indicates a hole or crack in the heat exchanger. This test can be done in conjunction with the flame rollout

component of the spillage test. Another method for conducting a flame distortion test is to slowly extend a match up and down into each combustion chamber with the burner off and the air handler fan on, and watch for movement of the flame head.

## **2. Blocked Flue Test**

With the furnace off, block the flue ports leading from the combustion chamber to the draft diverter or barometric damper. Squirt smoke into the combustion chamber. Turn on the furnace fan and watch to see if the smoke is disturbed when the fan comes on. Smoke movement indicates a hole or crack in the heat exchanger.

## **3. Tracer Gas Test**

A number of testing procedures exist for injecting a tracer gas into the combustion chamber (usually with the furnace fan off) and then measuring or detecting the tracer gas on the warm air side of the heat exchanger.

***If any of the above heat exchanger tests provides a positive indication for a cracked heat exchanger, immediate action should be taken to notify the residents of the potential danger, and a professional heating contractor should be contacted to investigate the problem.***

**Turn off fans and return appliance controls to their original settings once the test procedures have been completed.**

Special thanks to Advanced Energy, Sun Power and the Center for Energy and Environment (CEE) for their work in developing and refining the combustion safety test procedures above.

## Appendix A Calibration and Maintenance

### A.1 Fan Calibration Parameters (Updated January 2007)

#### Model 3 (110V) Calibration Parameters:

Fan Configuration	Calibration Parameters
Open Fan	Flow (cfm) = 506.8 x (Fan Pressure in Pa) <sup>.4879</sup>
Ring A Installed	Flow (cfm) = 190.1 x (Fan Pressure in Pa) <sup>.4876</sup>
Ring B Installed	Flow (cfm) = 60.67 x (Fan Pressure in Pa) <sup>.4955</sup>
Ring C Installed	Flow (cfm) = 21.37 x (Fan Pressure in Pa) <sup>.5132</sup>

#### Model 3 (230V) Calibration Parameters:

Fan Configuration	Calibration Parameters
Open Fan	Flow (cfm) = 498.9 x (Fan Pressure in Pa) <sup>.4918</sup>
Ring A Installed	Flow (cfm) = 190.1 x (Fan Pressure in Pa) <sup>.4889</sup>
Ring B Installed	Flow (cfm) = 60.35 x (Fan Pressure in Pa) <sup>.4958</sup>
Ring C Installed	Flow (cfm) = 20.47 x (Fan Pressure in Pa) <sup>.5178</sup>

#### Model 4 (230V) Calibration Parameters:

Fan Configuration	Calibration Parameters
Open Fan	Flow (cfm) = 438.7 x (Fan Pressure in Pa) <sup>.4848</sup>
Ring A Installed	Flow (cfm) = 160.8 x (Fan Pressure in Pa) <sup>.4952</sup>
Ring B Installed	Flow (cfm) = 48.08 x (Fan Pressure in Pa) <sup>.4968</sup>
Ring C Installed	Flow (cfm) = 11.36 x (Fan Pressure in Pa) <sup>.5157</sup>

**Note:** All fan flows indicated on Energy Conservatory gauges or flow tables are corrected to a standard air density of 0.075 lbs/cubic foot, and are not the actual volumetric flow going through the fan. The indicated flows are corrected to standard air density according to the CGSB Standard CAN/CG-SB-149.10-M86. The correction is done in such a way that, for particular types of leaks (where the viscosity of air is negligible and the flow exponent "n" equals 0.5), the indicated flow is independent of barometric pressure. For this type of leak, the indicated flow is the flow that would have been going through the fan if the building had been tested at standard barometric pressure, and indoor and outdoor temperatures were unchanged.

If the actual volumetric flow rate going through the fan is desired, multiply the indicated flow by:

$$\sqrt{\frac{0.075}{\text{actual air density}^*}} \quad (\text{where air density is in lb/ft}^3)$$

or

$$\sqrt{\frac{1.204}{\text{actual air density}^*}} \quad (\text{where air density is in Kg/m}^3)$$

\* Use the density of air flowing through the fan.

## **A.2 Issues Affecting Fan Calibration**


### ***A.2.a Fan Sensor and Motor Position:***

Model 3 and Model 4 Blower Door fans maintain their calibration unless physical damage occurs. Conditions which could cause the fan calibration to change are primarily damaged flow sensors, movement of the motor and blades relative to the fan housing, and leaks in the sensor or tubing running from the flow sensor to the fan pressure tap. These conditions are easily detected and should be tested for on a regular basis.


#### **Damaged Blower Door Flow Sensor**

Model 3 fans (both 110V and 230V) use a round white plastic flow sensor, while the Model 4 fan uses a flow sensor manufactured out of thin stainless steel tubing. The flow sensors are permanently attached to the end of the fan motor opposite the fan blades.

Model 3 Flow Sensor

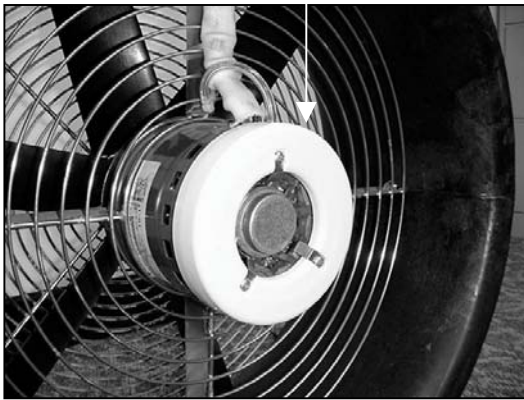

Model 4 Flow Sensor

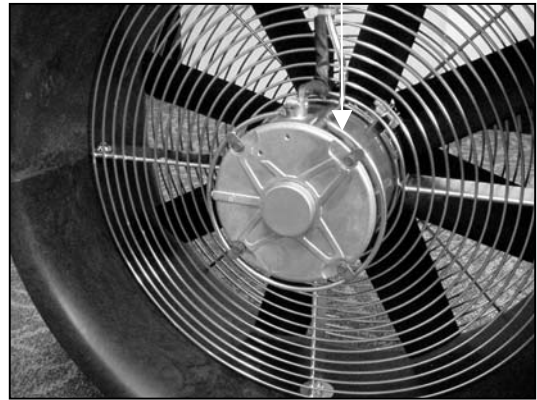

First visually confirm that the sensor is not broken or deformed due to impact. Check that the sensor is firmly attached to the motor. Next, perform a test for leaks in the sensor or the tubing connecting the sensor to the fan pressure tap (this test is easier if you first place the fan in an elevated position such as on a bench top or table.)

Attach a piece of tubing to the pressure tap on the Blower Door fan electrical box. Leave the other end of the tubing open. Find the 4 intentional pin holes in the flow sensor. For the Model 3 flow sensor they are evenly spaced around the outside rim of the sensor - for the Model 4 flow sensor they are evenly spaced on the back side of the sensor. Temporarily seal the 4 holes by covering them with masking tape. Next, create a vacuum in the fan pressure tubing by sucking on the open end. A vacuum in the tubing assures that the flow sensor does not leak. There is a vacuum, if by placing your tongue over the end of the tubing, the tubing sticks to your tongue. Make sure that the vacuum persists for at least 5 seconds. If a vacuum can not be created, contact The Energy Conservatory to further diagnose the sensor leakage problem.


#### **Blower Door Motor Position**

If a fan has been dropped, the motor may have shifted from its proper position in the motor mount. This can degrade the fan calibration. To test the motor position, lay the fan on its side with the flow sensor facing up and all Flow Rings removed. Place a straightedge (such as a heavy yardstick on edge) across the inlet of the fan. Use a ruler to measure the following distance and compare this measurement to the appropriate specification.

**Model 3 Fan:** Measure the distance from the bottom of the straightedge to the face of the flow sensor. This distance should be in the range of  $3/16^{\text{th}}$  to  $5/16^{\text{th}}$  of an inch. If the motor is not in the proper position, call The Energy Conservatory for further instructions.

**Model 4 Fan:** Measure the distance from the bottom of the straightedge to the face of the motor bearing cover. This distance should be in the range of  $3/8^{\text{th}}$  to  $5/8^{\text{th}}$  of an inch. If the motor is not in the proper position, call The Energy Conservatory for further instructions.

Figure 11: Schematic of Blower Door Fans

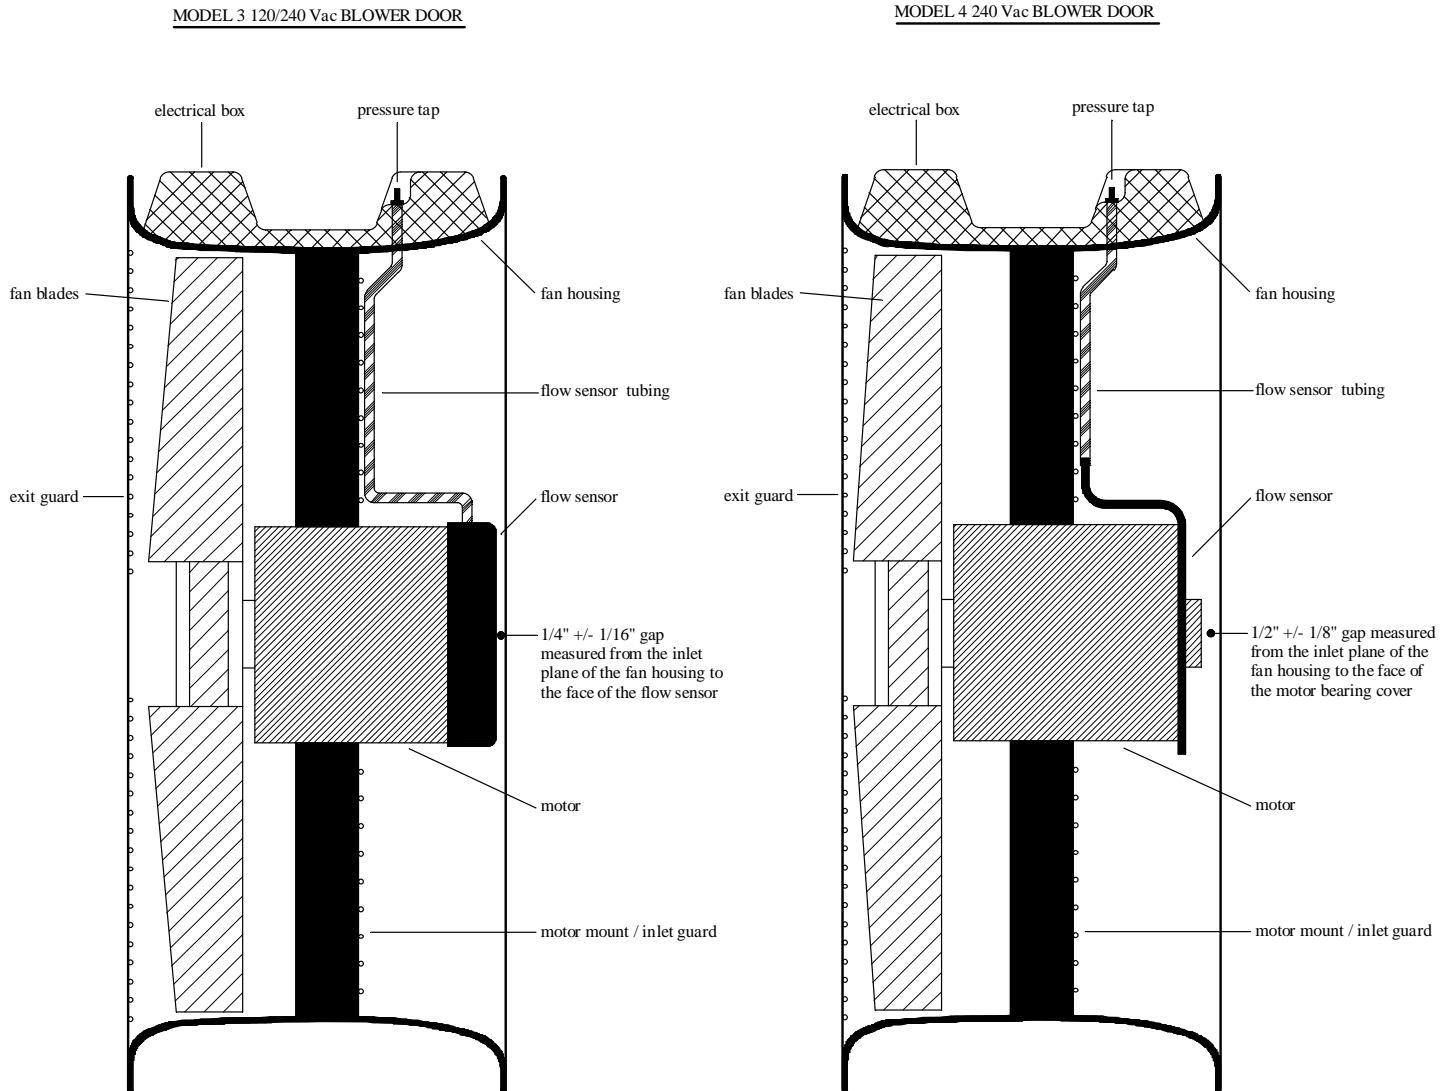

### ***A.2.b Upstream Air Flow Conditions:***

The calibration for all Blower Door fans are slightly sensitive to upstream air flow conditions (e.g. orientation of walls, doors, stairs etc. relative to the fan inlet). This is particularly true when measurements are taken using the “open fan” configuration. As a result, follow these simple rules whenever possible.

- It is always best to install the fan in a doorway leading to a large open room. Try to avoid installing the fan in a doorway where there are stairways or major obstructions to air flow very close (1-5 feet) to the fan inlet.
- If the fan must be installed next to a stairway or major obstruction, it is best to take measurements using one of the Flow Rings and not “open fan”.
- Always open the inside door and outside storm door as much as possible during the Blower Door test to prevent restrictions to air flow.

### ***A.2.c Operating Under High Backpressure Conditions:***

**Note:** For most testing applications, backpressure is not a concern and can be ignored.

The term “backpressure” is used to describe the pressure that the Blower Door fan is working against when it is running. Backpressure is determined by measuring the static pressure difference between the air directly upstream of the fan, and the air directly exiting the fan.

Under typical testing applications, the backpressure seen by the fan is simply the test pressure at which the building airtightness measurement is being measured made (e.g. 50 Pascals). However, there are applications where the Blower Door fan could see backpressures that are greater than the test pressure. For example, if the Blower Door fan is exhausting air into a confined area (such as an attached porch), it is possible that the porch area could become pressurized relative to outside creating a backpressure condition that is greater than the test pressure. Although the Blower Door's flow sensor was designed to be affected as little as possible by variations in backpressure, under certain high backpressure operating conditions (described below) the calibration of the fan can degrade.

#### **High Backpressure Conditions**

Model 3 and Model 4 Blower Door fans can be used in testing applications with backpressures up to 80 Pascals with no significant effect on calibration accuracy. This is true for all fan flow configurations (Open through Ring E), provided that the fan is operated within the accepted flow range for each configuration. Backpressures above 80 Pa can diminish the accuracy of the fan calibration and should be avoided.

### **A.3 Blower Door Fan Maintenance and Safety**

There are several maintenance tips and procedures to ensure the proper operation of the Blower Door fan and to avoid any safety risks.

#### ***A.3.a Maintenance Checks:***

- Examine the motor cooling holes for excessive dust build-up. Use a vacuum with a brush attachment to remove dust, or blow out the dust with compressed air.
- Inspect housing, blades and guards. Especially note clearance of blade tips relative to the fan housing. There should be about 1/4 inch of clearance.
- Inspect electrical wiring and electrical connections on the fan and the fan speed controller.

#### ***A.3.b General Operational Notes and Tips:***

- Do not reverse the fan (if the fan has a flow direction switch) while the blades are turning. Turn off the fan and wait for it to come to a complete stop before reversing the flow direction.
- For long-term operation, such as maintaining house pressure while air-sealing, use a Flow Ring whenever possible to ensure good airflow over the fan. This will minimize heating of the fan and is important in warmer weather.
- Do not run the fan for long periods of time in reverse.
- The motor is thermally protected and if you experience a motor shut down, be sure to turn off the fan speed controller so that the fan does not restart unexpectedly after the motor cools down.
- Make sure to press the power plug firmly into power receptacle on fan. Failure to do so can cause overheating of the power cord and possible damage.
- Do not use ungrounded outlets or adapter plugs.
- Do not operate if the motor, controller or any of the electrical connections are wet.

**The Blower Door Fan is a very powerful and potentially dangerous piece of equipment if not used and maintained properly.** Carefully examine the fan before each use. If the fan housing, fan guards, blade, controller or cords become damaged, do not operate the fan until repairs have been made. Keep people and pets away from the fan when it is operating. Contact The Energy Conservatory if there are any unusual noises or vibrations while the fan is running.

#### ***A.3.c Replacing the Model 4 Controller's Internal Fuse:***

##### **Diagnosing the Problem:**

If the Model 4 Blower Door fan stops running or fails to respond to speed commands:

- Verify that the fan speed controller is turned **ON**.
- Verify that the fan speed controller power cord is plugged into an AC power mains outlet.
- Verify that the AC power mains outlet has electrical power.
- Verify that the fan connect cord from the fan speed controller is plugged into the receptacle located on the fan electrical box.
- Turn the fan speed control knob from minimum to maximum and back to minimum. If the fan fails to respond then the internal fuse may be blown and need to be replaced.



**CAUTION – HAZARDOUS VOLTAGES INSIDE MODEL 4 SPEED CONTROLLER.**  
**UNPLUG POWER CORD FROM AC POWER MAINS OUTLET BEFORE SERVICING**  
**SPEED CONTROLLER.**


Replacement Fuse Specification – 5 Amp, 250VAC, 5 X 20 mm, FAST acting, approved by VDE/UL

**Opening the Model 4 Speed Controller Enclosure:**

- Verify the power cord is **not** plugged into an AC mains power and that the controller power switch is **OFF**.
- Remove the four screws attaching the bottom enclosure cover to the two endplates
- Carefully separate the bottom cover from the rest of the enclosure. Do not disconnect the green and yellow ground wire which connects the top and bottom halves of the enclosure.

**Replacing the Fuse:**

- Locate the terminal block fuse holder next to the printed circuit board and power line filter. See photo below for details.
- Firmly grasp the black handle of the fuse holder and pull out the old fuse.
- Carefully slip the old fuse out of the black handle. Insert the new fuse into the black handle.
- Align the rib on the black handle with the notch in the terminal block fuse holder.
- Press the black handle and new fuse back into the terminal block fuse holder.

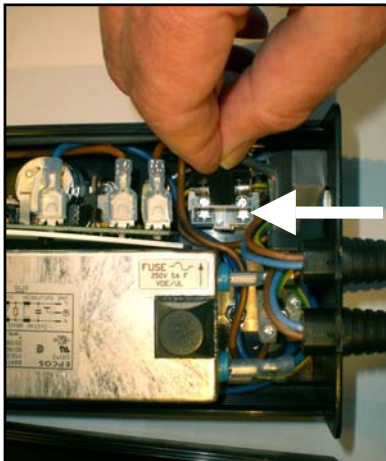

**Reassembling the Model 4 Speed Controller Enclosure:**

- Position the bottom enclosure cover in place between the two end plates.
- **CAUTION** – verify that no wires are being pinched as the enclosure is closed.
- Replace the four screws. With each screw, align the screw in its hole perpendicular to the end plate. Rotate the screw counterclockwise about one full turn until the threads drop into place.
- Tighten each screw and verify that each screw is tight.

**Verify Operation:**

- Reconnect the controller power cord to the AC power mains outlet.
- Turn **ON** the controller Power Switch.
- Adjust speed control knob from minimum to half speed and verify fan operation.
- Resume normal use of speed controller.

## **A.4 Calibration and Maintenance of Digital Pressure Gauges**

### ***A.4.a Digital Gauge Calibration:***

Re-calibration of digital pressure gauges is recommended every 12 months. Gauges should be sent back to The Energy Conservatory for re-calibration. It is also a good idea to perform gauge comparisons between calibrations, especially when damage is suspected (e.g. when a gauge has been dropped).

#### **Digital Gauge Comparison**

This technique is used to compare the readings of two digital gauges when they are both connected to the same pressure source. When two gauges are being compared, you should expect them to agree within their specifications:

##### DG-3 Accuracy Specifications:

Low Range:        +/- 1% of reading or 0.2 Pa, whichever is larger (0-200.0 Pa)  
 High Range:       +/- 1% of reading or 2 Pa, whichever is larger (0-800 Pa)  
                          +/- 2% of reading (800-1,000 Pa)

##### DG-700 Accuracy Specifications:

+/- 1% of reading or 0.15 Pa, whichever is greater (0-1,250 Pa)


#### **Parts Needed for Comparison**

- 2 digital gauges
- one Magnehelic gauge
- 2 “T” fittings
- one syringe
- five 1 foot sections of tubing

#### **Comparison Procedure**

Using the two T fittings and short sections of hose, hook up the gauges and syringe as shown in Figure 12 below. Turn on the digital gauges, (if DG-3's, set on High Range). They should both be reading 0 Pa. Pull out on the syringe slowly until the desired test pressure on the digital gauges is achieved. Record your results and compare with the specifications above.

Figure 12: Digital Gauge Comparison Setup

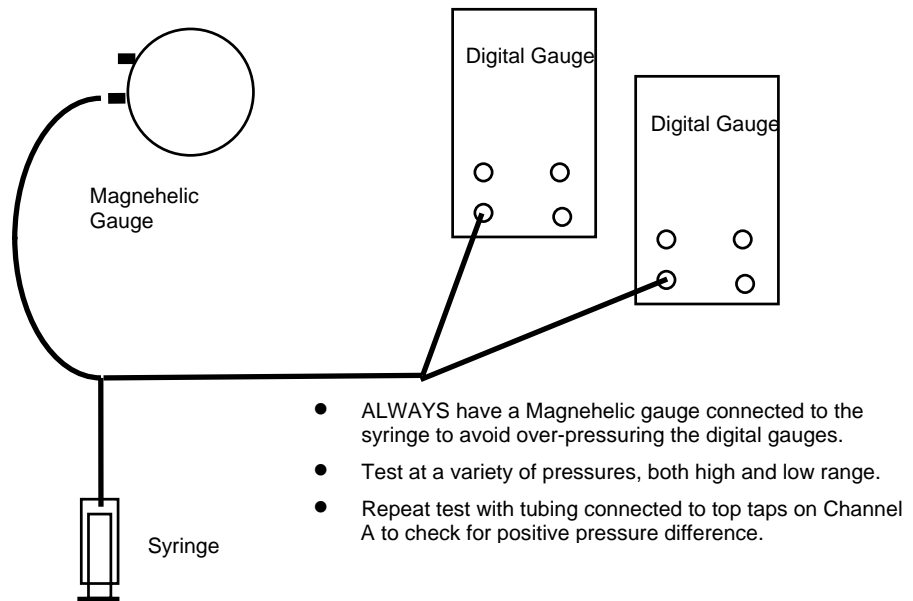

#### ***A.4.b Digital Gauge Maintenance:***

- Operating temperature range: 32 °F to 120 °F.
- Storage temperatures 5 °F to 160 °F (best to keep it warm during cold weather).
- Avoid conditions where condensation could occur, for example taking a gauge from a cool environment into a hot humid environment.
- Do not store gauge in the same container as chemical smoke. The smoke can and does cause corrosion.
- Do not ignore low battery indicator (readings can start being in error almost immediately).
- Avoid exposing the gauge to excessive pressures, such as caused by hoses slammed in a door.

### **A.5 Checking for Leaky Tubing**

It does not happen very often, but leaky tubing can seriously degrade the accuracy of Blower Door airtightness tests. These leaks can be small enough to go undetected for years but large enough to affect fan calibration.

- Before starting, inspect both ends of the tubing to make sure they are not stretched out to the point where they will not make a good seal when attached to a gauge.
- Seal off one end of the tubing by doubling it over on itself near the end.
- Create a vacuum in the tubing by sucking on the open end (make sure the hose is clean first!). Let the end of the tubing stick to your tongue due to the vacuum.
- The tubing should stick to your tongue indefinitely if there are no leaks. Waiting for 5 seconds or so is a good enough test.
- If the tubing has a leak, it should be replaced immediately.
- The ends of the tubing will sometimes get stretched out or torn after many uses. Periodically trim 1/4" off the ends of the tubing to remove the damaged end.

## Appendix B Flow Conversion Tables

### Model 3 (110V)

Flow (cfm)					Flow (cfm)				
Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C	Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
					122	5282	1978	656	251
					124	5324	1994	661	254
					126	5365	2010	666	256
					128	5407	2025	672	258
					130	5448	2041	677	260
					132	5489	2056	682	262
					134	5529	2071	687	264
					136	5569	2086	692	266
					138	5609	2101	697	268
					140	5648	2116	702	270
					142	5688	2130	707	272
					144	5727	2145	712	274
					146	5765	2159	717	276
					148	5804	2174	722	278
					150	5842	2188	726	280
					152	5880	2202	731	281
					154	5917	2216	736	283
					156	5955	2230	741	285
					158	5992	2244	745	287
					160	6029	2258	750	289
					162	6065	2272	755	291
					164	6102	2285	759	293
					166	6138	2299	764	294
					168	6174	2312	768	296
					170	6210	2326	773	298
					172	6245	2339	777	300
					174	6281	2352	782	302
					176	6316	2365	786	303
					178	6351	2378	791	305
					180	6385	2391	795	307
					182	6420	2404	799	309
					184	6454	2417	804	310
					186	6488	2430	808	312
					188	6522	2443	812	314
					190		2455	817	316
					192		2468	821	317
					194		2480	825	319
					196		2493	829	321
					198		2505	834	322
					200		2518	838	324
					202		2530	842	326
					204		2542	846	327
					206		2554	850	329
					208		2566	854	331
					210		2578	858	332
					212		2590	862	334
					214		2602	866	335
					216		2614	870	337
					218		2626	874	339
					220		2637	878	340
					222		2649	882	342
					224		2661	886	343
					226		2672	890	345
					228		2684	894	347
					230		2695	898	348
					232		2707	902	350
					234		2718	906	351
					236		2729	909	353
					238		2740	913	354
					240		2752	917	356
16				89					
18				94					
20				99					
22				104					
24				109					
26	2484	931	305	114					
28	2576	965	316	118					
30	2664	998	327	122					
32	2749	1030	338	127					
34	2832	1061	348	131					
36	2912	1091	358	134					
38	2990	1120	368	138					
40	3065	1149	377	142					
42	3139	1176	387	145					
44	3211	1203	396	149					
46	3282	1230	404	152					
48	3351	1255	413	156					
50	3418	1281	421	159					
52	3484	1305	430	162					
54	3549	1330	438	165					
56	3612	1353	446	169					
58	3675	1377	454	172					
60	3736	1400	461	175					
62	3796	1422	469	178					
64	3855	1444	476	181					
66	3914	1466	484	183					
68	3971	1488	491	186					
70	4028	1509	498	189					
72	4083	1530	505	192					
74	4138	1550	512	195					
76	4193	1571	519	197					
78	4246	1591	525	200					
80	4299	1610	532	202					
82	4351	1630	539	205					
84	4402	1649	545	208					
86	4453	1668	551	210					
88	4503	1687	558	213					
90	4553	1706	564	215					
92	4602	1724	570	218					
94	4651	1742	576	220					
96	4699	1760	582	222					
98	4746	1778	588	225					
100	4793	1796	594	227					
102	4840	1813	600	229					
104	4886	1830	606	232					
106	4932	1847	612	234					
108	4977	1864	617	236					
110	5021	1881	623	238					
112	5066	1898	629	241					
114	5110	1914	634	243					
116	5153	1930	640	245					
118	5196	1946	645	247					
120	5239	1962	650	249					



**Model 3 (110V)** Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
242		2763	921	357
244		2774	924	359
246		2785	928	360
248		2796	932	362
250		2807	936	363
252		2818	939	365
254		2829	943	366
256		2840	947	368
258		2850	950	369
260		2861	954	371
262		2872	958	372
264		2883	961	374
266		2893	965	375
268		2904	968	377
270		2914	972	378
272		2925	976	379
274		2935	979	381
276		2946	983	382
278		2956	986	384
280		2966	990	385
282		2977	993	387
284		2987	997	388
286		2997	1000	389
288		3007	1004	391
290		3018	1007	392
292		3028	1011	394
294		3038	1014	395
296		3048	1017	396
298		3058	1021	398
300		3068	1024	399
302		3078	1028	400
304		3088	1031	402
306		3098	1034	403
308		3108	1038	404
310		3117	1041	406
312		3127	1044	407
314		3137	1048	408
316		3147	1051	410
318		3156	1054	411
320		3166	1057	412
322		3176	1061	414
324		3185	1064	415
326		3195	1067	416
328		3204	1070	418
330		3214	1074	419
332		3223	1077	420
334		3233	1080	422
336		3242	1083	423
338		3252	1086	424
340		3261	1090	425
342		3270	1093	427
344		3280	1096	428
346		3289	1099	429
348		3298	1102	431
350		3307	1105	432
352		3317	1109	433
354		3326	1112	434
356		3335	1115	436
358		3344	1118	437
360		3353	1121	438
362		3362	1124	439
364		3371	1127	441
366		3380	1130	442
368		3389	1133	443
370		3398	1136	444

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
372		3407	1139	446
374		3416	1142	447
376		3425	1145	448
378		3434	1148	449
380		3443	1151	450
382		3452	1154	452
384		3460	1157	453
386		3469	1160	454
388		3478	1163	455
390		3487	1166	457
392		3495	1169	458
394		3504	1172	459
396		3513	1175	460
398		3521	1178	461
400		3530	1181	462
402		3538	1184	464
404		3547	1187	465
406		3556	1190	466
408		3564	1193	467
410		3573	1196	468
412		3581	1198	470
414		3590	1201	471
416		3598	1204	472
418		3606	1207	473
420		3615	1210	474
422		3623	1213	475
424		3632	1216	477
426		3640	1218	478
428		3648	1221	479
430		3657	1224	480
432		3665	1227	481
434		3673	1230	482
436		3681	1233	483
438		3690	1235	485
440		3698	1238	486
442		3706	1241	487
444		3714	1244	488
446		3722	1246	489
448		3730	1249	490
450		3739	1252	491
452		3747	1255	492
454		3755	1258	494
456		3763	1260	495
458		3771	1263	496
460		3779	1266	497
462		3787	1268	498
464		3795	1271	499
466		3803	1274	500
468		3811	1277	501
470		3819	1279	502
472		3827	1282	503
474		3834	1285	505
476		3842	1287	506
478		3850	1290	507
480		3858	1293	508
482		3866	1295	509
484		3874	1298	510
486		3882	1301	511
488		3889	1303	512
490		3897	1306	513
492		3905	1309	514
494		3913	1311	515
496		3920	1314	516
498		3928	1317	518
500		3936	1319	519



**Model 3 (230V)**

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
26	2477	935	304	111
28	2569	969	315	115
30	2657	1003	326	119
32	2743	1035	336	123
34	2826	1066	347	127
36	2907	1096	357	131
38	2985	1125	366	135
40	3061	1154	376	138
42	3136	1182	385	142
44	3208	1209	394	145
46	3279	1236	403	149
48	3348	1262	411	152
50	3416	1287	420	155
52	3483	1312	428	158
54	3548	1336	436	161
56	3612	1360	444	165
58	3675	1384	452	168
60	3737	1407	459	171
62	3797	1430	467	173
64	3857	1452	474	176
66	3916	1474	482	179
68	3974	1496	489	182
70	4031	1517	496	185
72	4087	1538	503	187
74	4143	1559	510	190
76	4197	1579	517	193
78	4251	1600	523	195
80	4305	1620	530	198
82	4357	1639	536	200
84	4409	1659	543	203
86	4460	1678	549	205
88	4511	1697	556	208
90	4561	1716	562	210
92	4611	1734	568	213
94	4660	1752	574	215
96	4708	1771	580	218
98	4756	1789	586	220
100	4804	1806	592	222
102	4851	1824	598	224
104	4897	1841	604	227
106	4944	1858	609	229
108	4989	1876	615	231
110	5034	1892	621	233
112	5079	1909	626	236
114	5124	1926	632	238
116	5168	1942	637	240
118	5211	1959	643	242
120	5255	1975	648	244

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
122	5297	1991	653	246
124	5340	2007	659	248
126	5382	2022	664	250
128	5424	2038	669	252
130	5466	2053	674	255
132	5507	2069	679	257
134	5548	2084	684	259
136	5588	2099	689	261
138	5628	2114	694	263
140	5668	2129	699	264
142	5708	2144	704	266
144	5747	2159	709	268
146	5787	2173	714	270
148	5825	2188	719	272
150	5864	2202	724	274
152	5902	2217	729	276
154	5940	2231	733	278
156	5978	2245	738	280
158	6016	2259	743	282
160	6053	2273	747	283
162	6090	2287	752	285
164	6127	2300	756	287
166	6164	2314	761	289
168	6200	2328	766	291
170	6236	2341	770	292
172	6272	2355	775	294
174	6308	2368	779	296
176	6344	2381	783	298
178	6379	2394	788	299
180	6414	2408	792	301
182	6449	2421	797	303
184	6484	2434	801	305
186	6518	2447	805	306
188	6553	2459	809	308
190		2472	814	310
192		2485	818	311
194		2497	822	313
196		2510	826	315
198		2522	831	316
200		2535	835	318
202		2547	839	320
204		2560	843	321
206		2572	847	323
208		2584	851	325
210		2596	855	326
212		2608	859	328
214		2620	863	329
216		2632	867	331
218		2644	871	333
220		2656	875	334
222		2668	879	336
224		2679	883	337
226		2691	887	339
228		2703	891	340
230		2714	895	342
232		2726	898	344
234		2737	902	345
236		2749	906	347
238		2760	910	348
240		2771	914	350



**Model 3 (230V)** Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
242		2782	917	351
244		2794	921	353
246		2805	925	354
248		2816	929	356
250		2827	932	357
252		2838	936	359
254		2849	940	360
256		2860	943	361
258		2871	947	363
260		2882	951	364
262		2893	954	366
264		2903	958	367
266		2914	961	369
268		2925	965	370
270		2935	969	372
272		2946	972	373
274		2957	976	374
276		2967	979	376
278		2978	983	377
280		2988	986	379
282		2999	990	380
284		3009	993	381
286		3019	997	383
288		3030	1000	384
290		3040	1004	386
292		3050	1007	387
294		3060	1010	388
296		3070	1014	390
298		3081	1017	391
300		3091	1021	392
302		3101	1024	394
304		3111	1027	395
306		3121	1031	396
308		3131	1034	398
310		3141	1037	399
312		3150	1041	400
314		3160	1044	402
316		3170	1047	403
318		3180	1050	404
320		3190	1054	406
322		3199	1057	407
324		3209	1060	408
326		3219	1063	410
328		3228	1067	411
330		3238	1070	412
332		3248	1073	414
334		3257	1076	415
336		3267	1080	416
338		3276	1083	417
340		3286	1086	419
342		3295	1089	420
344		3305	1092	421
346		3314	1095	423
348		3323	1098	424
350		3333	1102	425
352		3342	1105	426
354		3351	1108	428
356		3360	1111	429
358		3370	1114	430
360		3379	1117	431
362		3388	1120	433
364		3397	1123	434
366		3406	1126	435
368		3415	1129	436
370		3424	1132	437

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
372		3433	1135	439
374		3442	1138	440
376		3451	1141	441
378		3460	1144	442
380		3469	1147	444
382		3478	1150	445
384		3487	1153	446
386		3496	1156	447
388		3505	1159	448
390		3514	1162	450
392		3522	1165	451
394		3531	1168	452
396		3540	1171	453
398		3549	1174	454
400		3557	1177	455
402		3566	1180	457
404		3575	1183	458
406		3583	1186	459
408		3592	1189	460
410		3601	1192	461
412		3609	1194	462
414		3618	1197	464
416		3626	1200	465
418		3635	1203	466
420		3643	1206	467
422		3652	1209	468
424		3660	1212	469
426		3669	1214	471
428		3677	1217	472
430		3685	1220	473
432		3694	1223	474
434		3702	1226	475
436		3710	1228	476
438		3719	1231	477
440		3727	1234	479
442		3735	1237	480
444		3744	1240	481
446		3752	1242	482
448		3760	1245	483
450		3768	1248	484
452		3776	1251	485
454		3785	1253	486
456		3793	1256	487
458		3801	1259	489
460		3809	1261	490
462		3817	1264	491
464		3825	1267	492
466		3833	1270	493
468		3841	1272	494
470		3849	1275	495
472		3857	1278	496
474		3865	1280	497
476		3873	1283	498
478		3881	1286	499
480		3889	1288	501
482		3897	1291	502
484		3905	1294	503
486		3913	1296	504
488		3921	1299	505
490		3928	1302	506
492		3936	1304	507
494		3944	1307	508
496		3952	1309	509
498		3960	1312	510
500		3967	1315	511



**Model 4 (230V)**

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
16				47
18				50
20			213	53
22			223	56
24			233	58
26	2129	807	243	61
28	2207	837	252	63
30	2282	866	261	66
32	2354	895	269	68
34	2425	922	277	70
36	2493	948	285	72
38	2559	974	293	74
40	2623	999	301	76
42	2686	1024	308	78
44	2747	1047	315	80
46	2807	1071	322	82
48	2866	1094	329	84
50	2923	1116	336	85
52	2979	1138	342	87
54	3034	1159	349	89
56	3088	1180	355	91
58	3141	1201	361	92
60	3193	1221	368	94
62	3244	1241	374	95
64	3295	1261	380	97
66	3344	1280	385	99
68	3393	1299	391	100
70	3441	1318	397	102
72	3488	1337	402	103
74	3535	1355	408	105
76	3581	1373	413	106
78	3626	1391	419	107
80	3671	1408	424	109
82	3715	1426	429	110
84	3759	1443	434	112
86	3802	1460	440	113
88	3845	1476	445	114
90	3887	1493	450	116
92	3928	1509	455	117
94	3970	1525	459	118
96	4010	1541	464	120
98	4051	1557	469	121
100	4090	1573	474	122
102	4130	1588	478	123
104	4169	1604	483	125
106	4208	1619	488	126
108	4246	1634	492	127
110	4284	1649	497	128
112	4321	1664	501	129
114	4359	1678	506	131
116	4396	1693	510	132
118	4432	1707	514	133
120	4468	1721	519	134

Flow (cfm)

Fan Pressure (Pa)	Open Fan	Ring A	Ring B	Ring C
122	4504	1736	523	135
124	4540	1750	527	136
126	4575	1764	531	138
128	4610	1777	536	139
130	4645	1791	540	140
132	4680	1805	544	141
134	4714	1818	548	142
136	4748	1832	552	143
138	4782	1845	556	144
140	4815	1858	560	145
142	4848	1871	564	146
144	4881	1884	568	147
146	4914	1897	572	148
148	4947	1910	576	149
150	4979	1923	580	150
152	5011	1935	583	152
154	5043	1948	587	153
156	5075	1960	591	154
158	5106	1973	595	155
160	5137	1985	598	156
162	5168	1997	602	157
164	5199	2009	606	158
166	5230	2022	609	159
168	5260	2034	613	160
170	5290	2046	617	161
172	5320	2057	620	161
174	5350	2069	624	162
176	5380	2081	627	163
178	5410	2093	631	164
180	5439	2104	634	165
182	5468	2116	638	166
184	5497	2127	641	167
186	5526	2139	645	168
188	5555	2150	648	169
190		2161	652	170
192		2173	655	171
194		2184	659	172
196		2195	662	173
198		2206	665	174
200		2217	669	175
202		2228	672	175
204		2239	675	176
206		2250	678	177
208		2260	682	178
210		2271	685	179
212		2282	688	180
214		2292	691	181
216		2303	695	182
218		2314	698	182
220		2324	701	183
222		2335	704	184
224		2345	707	185
226		2355	710	186
228		2366	714	187
230		2376	717	188
232		2386	720	188
234		2396	723	189
236		2406	726	190
238		2416	729	191
240		2426	732	192



**Model 4 (230V)** Flow (cfm)

Fan Pressure	Open Fan	Ring A	Ring B	Ring C
242		2436	735	193
244		2446	738	193
246		2456	741	194
248		2466	744	195
250		2476	747	196
252		2486	750	197
254		2496	753	197
256		2505	756	198
258		2515	759	199
260		2525	762	200
262		2534	765	201
264		2544	767	201
266		2553	770	202
268		2563	773	203
270		2572	776	204
272		2582	779	205
274		2591	782	205
276		2600	785	206
278		2610	787	207
280		2619	790	208
282		2628	793	208
284		2637	796	209
286		2647	799	210
288		2656	801	211
290		2665	804	211
292		2674	807	212
294		2683	810	213
296		2692	812	214
298		2701	815	214
300		2710	818	215
302		2719	820	216
304		2728	823	217
306		2737	826	217
308		2745	829	218
310		2754	831	219
312		2763	834	220
314		2772	836	220
316		2781	839	221
318		2789	842	222
320		2798	844	222
322		2807	847	223
324		2815	850	224
326		2824	852	225
328		2832	855	225
330		2841	857	226
332		2849	860	227
334		2858	863	227
336		2866	865	228
338		2875	868	229
340		2883	870	230
342		2892	873	230
344		2900	875	231
346		2908	878	232
348		2917	880	232
350		2925	883	233
352		2933	885	234
354		2941	888	234
356		2950	890	235
358		2958	893	236
360		2966	895	236
362		2974	898	237
364		2982	900	238
366		2990	903	238
368		2998	905	239
370		3006	908	240

Flow (cfm)

Fan Pressure	Open Fan	Ring A	Ring B	Ring C
372		3015	910	240
374		3023	912	241
376		3031	915	242
378		3039	917	242
380		3046	920	243
382		3054	922	244
384		3062	924	244
386		3070	927	245
388		3078	929	246
390		3086	932	246
392		3094	934	247
394		3102	936	248
396		3109	939	248
398		3117	941	249
400		3125	943	250
402		3133	946	250
404		3140	948	251
406		3148	950	251
408		3156	953	252
410		3163	955	253
412		3171	957	253
414		3179	960	254
416		3186	962	255
418		3194	964	255
420		3201	967	256
422		3209	969	257
424		3216	971	257
426		3224	973	258
428		3231	976	258
430		3239	978	259
432		3246	980	260
434		3254	982	260
436		3261	985	261
438		3268	987	262
440		3276	989	262
442		3283	991	263
444		3291	994	263
446		3298	996	264
448		3305	998	265
450		3313	1000	265
452		3320	1002	266
454		3327	1005	266
456		3334	1007	267
458		3342	1009	268
460		3349	1011	268
462		3356	1013	269
464		3363	1016	269
466		3370	1018	270
468		3377	1020	271
470		3385	1022	271
472		3392	1024	272
474		3399	1026	272
476		3406	1029	273
478		3413	1031	274
480		3420	1033	274
482		3427	1035	275
484		3434	1037	275
486		3441	1039	276
488		3448	1041	277
490		3455	1043	277
492		3462	1046	278
494		3469	1048	278
496		3476	1050	279
498		3483	1052	279
500		3490	1054	280




## Appendix C Using Flow Rings C, D and E

### C.1 Using Ring C

Ring C is used with the Model 3 Minneapolis Blower Door system to measure fan flows between 300 and 85 cfm, and between 260 and 50 cfm with the Model 4 system. Flows in this range are typically measured in very tightly constructed new houses, or in airtight rooms (e.g. computer rooms).

#### C.1.a Installation:

To install **Ring C**, place Ring C in the center of Ring B and rotate the 6 fastener clips attached to Ring B so that they rotate over the edge of Ring C and secure it in place.

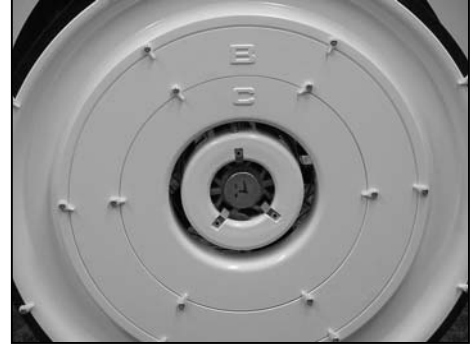

#### C.1.b Calibration Parameters for Ring C (Updated January 2007):

Model 3 (110V):	Flow (cfm) = 21.37 x (Fan Pressure in Pa) <sup>-0.5132</sup>
Model 3 (230V):	Flow (cfm) = 20.47 x (Fan Pressure in Pa) <sup>-0.5178</sup>
Model 4 (230V):	Flow (cfm) = 11.36 x (Fan Pressure in Pa) <sup>-0.5157</sup>

A flow conversion table for Ring C can be found in Appendix B.


### C.2 Using Rings D and E

Rings D and E have been designed to measure very low air flows with Model 3 and 4 Minneapolis Blower Door systems. Ring D has a flow range between 125 and 30 cfm. Ring E has a flow range between 50 and 11 cfm.

#### C.2.a Installation:

##### Ring D

**Ring D** attaches directly to the center of Ring B and is secured by the 6 rotating fastener clips found on Ring B. Install Ring D so that the letter “D” is in the “12 o’clock” position.


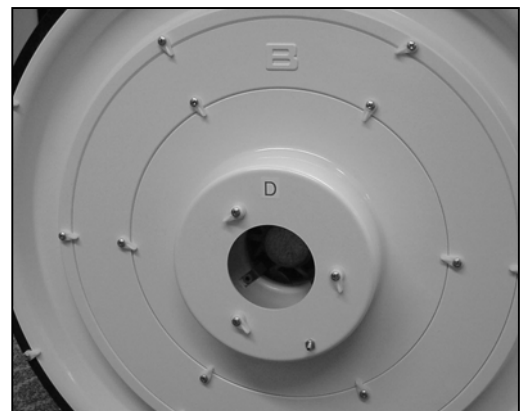


### Ring E

**Ring E** attaches directly to the center of Ring D and is secured by the 3 rotating fastener clips found on Ring D. Install Ring E so that the letter "E" is in the "12 o'clock" position.

#### C.2.b Measuring Fan Flow with Rings D and E:

When using either Rings D or E, it is necessary to measure fan pressure by using the pressure tap mounted directly on Ring D, rather than the pressure tap located on the top of the fan.

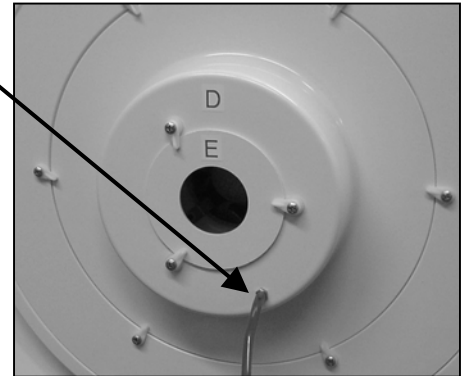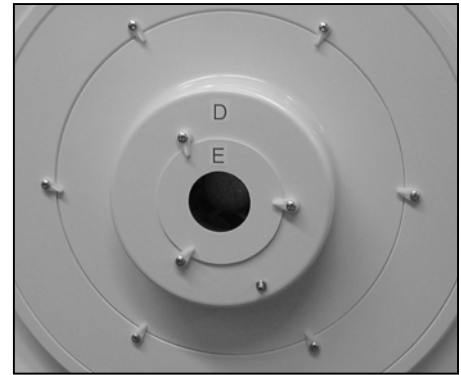

#### C.2.c Calibration Parameters for Rings D and E (Updated January 2007):

Ring D:	Model 3 (110V):	Flow (CFM) = 7.216 x (Fan Pressure in Pa) <sup>.4942</sup>
	Model 3 (230V):	Flow (CFM) = 6.870 x (Fan Pressure in Pa) <sup>.5022</sup>
	Model 4 (230V):	Flow (CFM) = 7.246 x (Fan Pressure in Pa) <sup>.5032</sup>
Ring E:	Model 3 (110V):	Flow (CFM) = 2.726 x (Fan Pressure in Pa) <sup>.5267</sup>
	Model 3 (230V):	Flow (CFM) = 2.817 x (Fan Pressure in Pa) <sup>.5139</sup>
	Model 4 (230V):	Flow (CFM) = 2.802 x (Fan Pressure in Pa) <sup>.5166</sup>

A flow conversion table for Rings D and E is presented below:

**Note:** If you are using Rings C, D or E with an older set of Flow Rings that have 3 fastening washers instead of the 6 rotating fastener clips, you should temporarily tape the following locations to prevent air leakage between the Rings.

- the outer edge between Ring A and the fan housing.
- the edge (joint) between Ring B and Ring A.
- the edge (joint) between Ring C and Ring B.
- the edge (joint) between Ring D and Ring B.

Flow Conversion Table for Rings D and E (Model 3 (110V))

Flow (cfm)			
Fan Pressure (Pa)	Low-Flow Ring D	Low-Flow Ring E	
15	28	11	
20	32	13	
25	35	15	
30	39	16	
35	42	18	
40	45	19	
45	47	20	
50	50	21	
55	52	22	
60	55	24	
65	57	25	
70	59	26	
75	61	26	
80	63	27	
85	65	28	
90	67	29	
95	68	30	
100	70	31	

Flow (cfm)			
Fan Pressure (Pa)	Low-Flow Ring D	Low-Flow Ring E	
105	72	32	
110	74	32	
115	75	33	
120	77	34	
125	78	35	
130	80	35	
135	81	36	
140	83	37	
145	84	37	
150	86	38	
155	87	39	
160	89	39	
165	90	40	
170	91	41	
175	93	41	
180	94	42	
185	95	43	
190	96	43	

Flow (cfm)			
Fan Pressure (Pa)	Low-Flow Ring D	Low-Flow Ring E	
195	98	44	
200	99	44	
205	100	45	
210	101	46	
215	103	46	
220	104	47	
225	105	47	
230	106	48	
235	107	48	
240	108	49	
245	109	49	
250	110	50	
255	112	50	
260	113	51	
265	114	52	
270	115	52	
275	116	53	
280	117	53	
290	119	54	
295	120	54	

Flow (cfm)			
Fan Pressure (Pa)	Low-Flow Ring D	Low-Flow Ring E	
300	121	55	
305	122	55	
310	123	56	
315	124	56	
320	125	57	

## ***Appendix D*   Sample Test Forms**

# Building Airtightness Test Form

## Customer Information:

Name: Tom Jones  
 Address: 2345 First ave.  
 City: Minneapolis  
 State/Zip: MN, 55444  
 Phone: 612-566-6000  
 Email: tjones@wildworld.com

## Building and Test Conditions:

Date: Jan 1, 2000  
 Time: 1:00 PM  
 Indoor Temperature (F): 70  
 Outdoor Temperature (F): 20  
 Volume (ft<sup>3</sup>): 22000  
 Floor Area (ft<sup>2</sup>): 2800  
 Surface Area (ft<sup>2</sup>): 3000  
 # Bedrooms: 4  
 # Occupants: 4  
 Wind Shielding: Moderate

## Building Address: (if different from above)

Street: \_\_\_\_\_  
 City/State: \_\_\_\_\_

## Comments:

Owner complains of condensation on windows.  
 Crawl space is wet.  
 2 smokers in the house.  
 Downspouts dump directly at the base of the house.

## Test #1

Depress x Press \_\_\_\_\_

Pre-test Baseline Pressure: 0 (Pa) Mag Gauges

Bldg Press. (Pa)	Flow Ring Installed	Fan Press (Pa)	Flow (cfm)
-55	Open	73	4091
-50	Open	65	3862
-44	Open	56	3588
-38	Open	45	3220
-30	Open	33	2762
-26	Open	26	2455
-15	Ring A	100	1764

Post-test Baseline Pressure: NA (Pa)

Fan Model/SN: Model 3 S/N 8331

## Results: (from TECTITE Program)

CFM50: 3674  
 ACH50: 10.0  
 CFM50/ft<sup>2</sup>: 1.3  
 Mpls Leakage Ratio: 1.2

## Test #2

Depress \_\_\_\_\_ Press \_\_\_\_\_

Pre-test Baseline Pressure: \_\_\_\_\_ (Pa)

Bldg Press. (Pa)	Flow Ring Installed	Fan Press (Pa)	Flow (cfm)

Post-test Baseline Pressure: \_\_\_\_\_ (Pa)

Fan Model/SN: \_\_\_\_\_

## Results:

CFM50: \_\_\_\_\_  
 ACH50: \_\_\_\_\_  
 CFM50/ft<sup>2</sup>: \_\_\_\_\_  
 Mpls Leakage Ratio: \_\_\_\_\_

# Building Airtightness Test Form

## Customer Information:

Name: \_\_\_\_\_  
 Address: \_\_\_\_\_  
 City: \_\_\_\_\_  
 State/Zip: \_\_\_\_\_  
 Phone: \_\_\_\_\_  
 Email: \_\_\_\_\_

## Building Address: (if different from above)

Street: \_\_\_\_\_  
 City/State: \_\_\_\_\_

## Building and Test Conditions:

Date: \_\_\_\_\_  
 Time: \_\_\_\_\_  
 Indoor Temperature (F): \_\_\_\_\_  
 Outdoor Temperature (F): \_\_\_\_\_  
 Volume (ft<sup>3</sup>): \_\_\_\_\_  
 Floor Area (ft<sup>2</sup>): \_\_\_\_\_  
 Surface Area (ft<sup>2</sup>): \_\_\_\_\_  
 # Bedrooms: \_\_\_\_\_  
 # Occupants: \_\_\_\_\_  
 Wind Shielding: \_\_\_\_\_

## Comments:

\_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_

## Test #1

Depress \_\_\_\_\_ Press \_\_\_\_\_

Pre-test Baseline Pressure: \_\_\_\_\_ (Pa)

Bldg Press. (Pa)	Flow Ring Installed	Fan Press (Pa)	Flow (cfm)

Post-test Baseline Pressure: \_\_\_\_\_ (Pa)

Fan Model/SN: \_\_\_\_\_

## Results:

CFM50: \_\_\_\_\_  
 ACH50: \_\_\_\_\_  
 CFM50/ft<sup>2</sup>: \_\_\_\_\_  
 Mpls Leakage Ratio: \_\_\_\_\_

## Test #2

Depress \_\_\_\_\_ Press \_\_\_\_\_

Pre-test Baseline Pressure: \_\_\_\_\_ (Pa)

Bldg Press. (Pa)	Flow Ring Installed	Fan Press (Pa)	Flow (cfm)

Post-test Baseline Pressure: \_\_\_\_\_ (Pa)

Fan Model/SN: \_\_\_\_\_

## Results:

CFM50: \_\_\_\_\_  
 ACH50: \_\_\_\_\_  
 CFM50/ft<sup>2</sup>: \_\_\_\_\_  
 Mpls Leakage Ratio: \_\_\_\_\_

## Appendix E Home Energy Article \*

### Infiltration: Just ACH50 Divided by 20?

by Alan Meier

*Alan Meier is executive editor of Home Energy Magazine.*

*This Home Energy classic, originally printed in 1986, explains a simple way to take one air infiltration measurement and determine a home's average air infiltration rate.*

Many researchers have sought to develop a correlation between a one-time pressurization test and an annual infiltration rate. Translating blower door measurements into an average infiltration rate has bedeviled the retrofitter and researcher alike. The rate of air infiltration constantly varies, yet the pressurization test is typically a single measurement. Nevertheless, many researchers have sought to develop a correlation between a one-time pressurization test and an annual infiltration rate.

#### ACH Divided by 20

In the late 1970s, a simple relation between a one-time pressurization test and an average infiltration rate grew out of experimentation at Princeton University. For a few years, the correlation remained "Princeton folklore" because no real research supported the relationship. In 1982, J. Kronvall and Andrew Persily compared pressurization tests to infiltration rates measured with tracer-gas for groups of houses in New Jersey and Sweden. They focused on pressurization tests at 50 Pascals because this pressure was already used by the Swedes and Canadians in their building standards. (This measurement is typically called "ACH50.") Other countries and groups within the United States have also adopted ACH as a measure of house tightness. Persily (now at the National Institute of Science and Technology) obtained a reasonably good estimate of average infiltration rates by dividing the air change rates at 50 Pascals by 20, that is:

$$\text{average infiltration rate (ACH)} = \frac{\text{ACH50}(1)}{20}$$

In this formula, ACH50 denotes the hourly air change rate at a pressure difference of 50 Pascals between inside and outside. Thus, for a house with 15 ACH at 50 Pascals (ACH50 = 15), one would predict an average air change rate of  $(15/20 = )$  0.75 ACH.

This simple formula yields surprisingly reasonable average infiltration estimates, even though it ignores many details of the infiltration process. These "details" are described below:

\* Printed by Permission of Home Energy Magazine.



- **Stack effect.** Rising warm air induces a pressure difference, or "stack effect," that causes exfiltration through the ceiling and infiltration at (or below) ground level. The stack effect depends on both the outside temperature and the height of the building. A colder outside temperature will cause a stronger stack effect. Thus, given two identically tall buildings, the one located in a cold climate will have more stack-induced infiltration. A taller building will also have a larger stack effect. Even though outside temperature and building height affect average infiltration rates, neither is measured by the pressure test. During the summer, stack effects disappear because the inside air is usually cooler (especially when the air conditioner is operating). Wind-induced pressure therefore becomes the dominant infiltration path.
- **Windiness and wind shielding.** Wind is usually the major driving force in infiltration, so it is only reasonable to expect higher infiltration rates in windy areas. Thus, given two identical buildings, the one located in a windy location will have more wind-induced infiltration. Nevertheless, a correlation such as ACH50/20 does not include any adjustment for windiness at the house's location. Trees, shrubs, neighboring houses, and other materials also shield a house from the wind's full force. Since a brisk wind can easily develop 10 Pascals on a windward wall, the extent of shielding can significantly influence total infiltration. A pressurization test does not directly measure the extent of shielding (although a house with good shielding may yield more accurate measurements since it is less affected by wind).
- **Type of leaks.** The leakage behavior of a hole in the building envelope varies with the shape of the hole. A long thin crack, for example, responds less to variations in air pressure than a round hole does. The pressure/air change curve (determined with a calibrated blower door) often gives clues to the types of leaks in a house.

A person conducting pressurization tests on a particular house can collect considerable information about these details. For example, it is easy to measure a house's height and estimate the wind exposure. The kinds of cracks can often be judged through careful inspection of the building construction. Climate data, including windiness and temperature, can be obtained from local weather stations. Ideally, this additional information should be applied to the formula in order to get a correlation factor more accurate for that house. Unfortunately, the formula was developed from data in just a few houses in New Jersey and Sweden, and it cannot be easily adjusted to other locations and circumstances. Should a retrofitter in Texas also use ACH50/20, or is dividing by 15 more appropriate for the Texas climate and house construction types?

### The LBL Infiltration Model

Researchers at Lawrence Berkeley Laboratory developed a model to convert a series of fan pressurization measurements into an "equivalent leakage area." (See HE, "Blower Doors: Infiltration Is Where the Action Is," Mar/Apr. '86, p.6. and the ASHRAE Book of Fundamentals chapter on ventilation and infiltration.) The equivalent leakage area roughly corresponds to the combined area of all the house's leaks.



A second formula converts the equivalent leakage area into an average infiltration rate in air changes per hour. This formula combines the physical principles causing infiltration with a few subjective estimates of building characteristics, to create relatively robust estimates of infiltration. ASHRAE has approved the technique and describes the formulae in ASHRAE Fundamentals. The LBL infiltration model is now the most commonly accepted procedure for estimating infiltration rates.

Max Sherman at LBL used this model to derive the theoretical correlation between pressure tests at 50 Pascals and annual average infiltration rates.<sup>1</sup> His major contribution was to create a climate factor to reflect the influence of outside temperature (which determines the stack effect) and windiness. Sherman estimated the climate factor using climate data for North America and plotted it (see Figure 1). Since the factor reflects both temperature and seasonal windiness, a cold, calm location could have the same climate factor as a warm, windy location. The map also reflects summer infiltration characteristics. Note how Texas and Vermont have the same climate factors.

Sherman found that the correlation factor in the revised formula could be expressed as the product of several factors:

$$\text{correlation factor, } N = C * H * S * L \quad (2)$$

where:

C = climate factor, a function of annual temperatures and wind (see Figure 1)

H = height correction factor (see Table 1)

S = wind shielding correction factor (see Table 2)

L = leakiness correction factor (see Table 3)

Values for each of the factors can be selected by consulting Figure 1 and Tables 1-3. An estimate of the average annual infiltration rate is thus given by

$$\text{average air changes per hour} = \frac{\text{ACH50}}{N} \quad (3)$$

This formula provides a more customized "rule-of-thumb" than the original ACH50/20, when additional information about the house is available.

### An Example

The application of the climate correction is best shown in an example. Suppose you are pressure testing a new, low-energy house in Rapid City, South Dakota. It is a two-story house, on an exposed site, with no surrounding vegetation or nearby houses to protect it from the wind.

1. At 50 Pascals, you determine that the ACH50 is 14.
  2. You consult Figure 1, and determine that the house has a climate factor, "C," of 14-17. Since Rapid City is near a higher contour line, select 17.
  3. The house is two stories tall, so the appropriate height correction factor, "H" (from Table 1), is 0.8.
  4. The house is very exposed to wind, and there are no neighboring houses or nearby trees and shrubs. The appropriate wind shielding correction factor, "S" (from Table 2), is 0.9.
  5. The house is new, and presumably well-built. The appropriate leakiness factor, "L" (from Table 3), is 1.4.
6. Calculate N:

$$\begin{aligned}
 N &= 17 * 0.8 * 0.9 * 1.4 \\
 &= 17
 \end{aligned}$$

Calculate the average annual infiltration rate:

$$\begin{aligned}
 \text{ACH} &= \frac{\text{ACH50}}{17} \\
 &= \frac{14}{17} \\
 &= 0.82
 \end{aligned}$$

The difference in this case (between dividing by 20 and 17) is not great--only 17%--but it demonstrates how the building conditions and location can affect the interpretation of pressurization tests.

Sherman compared his results to those reported by Persily. Sherman noted that he obtained a correlation factor (N) of about 20 for a typical house in the New Jersey area. Thus, Sherman's theoretically derived correlation factor yields results similar to Persily's empirically derived correlation factor.

The range of adjustment can be quite large. In extreme cases, the correlation factor, N, can be as small as 6, and as large as 40. In other words, the ACH50/20 rule of thumb could overestimate infiltration by a factor of two, or underestimate it by a factor of about three. This formula is still only a theory; it has not been validated with field measurements. Moreover, there is considerable controversy regarding the physical interpretation of the climate factor. For example, the formula yields a year-round average infiltration rate, rather than just for the heating season. Such a result is useful for houses with both space heating and cooling, but it may be misleading for some areas.

## Recommendations

There is no simple way to accurately convert a single pressure-test of a building to an average infiltration rate, because many building and climate-dependent factors affect true infiltration. Long-term tracer gas measurements are the only reliable way to obtain average infiltration rates. However, tracer gas measurements are impractical for retrofitters, and even most conservation researchers. A simplified rule of thumb to let the retrofitter quickly translate a pressure-test to an infiltration rate is clearly attractive.

Persily and Kronvall developed a crude conversion technique, ACH50/20, that provides reasonable results. On the other hand, it was impossible to customize the relationship of ACH50/20 to local conditions. What are the components of the magic number, 20?

Now Sherman has created a similar conversion factor that can be modified to reflect local building and climate conditions. This correlation factor accounts for windiness, climate, stack effect, and construction quality. Some judgement is needed to select the appropriate correction factors, but the blower-door user can now understand the quantitative impact of local conditions on infiltration. For example, a three-story house will have significantly more infiltration than a ranch house--even though the pressure tests are identical--due to a greater stack effect. (Clearly an infiltration standard should take these factors into account.)

Of course, Sherman's correlation factor still cannot account for occupant behavior or perversities in the building's construction. Nor is it a substitute for tracer-gas measurements. Field measurements must also be conducted to validate the formula. Still, it puts a scientific foundation behind what was previously an empirically derived relationship. It is a modest step forward in the efficient and accurate use of the blower door.

---

**Table 1. Height Correction Factor**

*Select the most appropriate value and insert in Equation 2.*

Number of stories	1	1.5	2	3
Correction factor "H"	1.0	0.9	0.8	0.7

---

**Table 2. Wind Shielding Correction Factor**

*Select the most appropriate value and insert in Equation 2.*

Extent of shielding	well-shielded	normal	exposed
Correction factor "S"	1.2	1.0	0.9

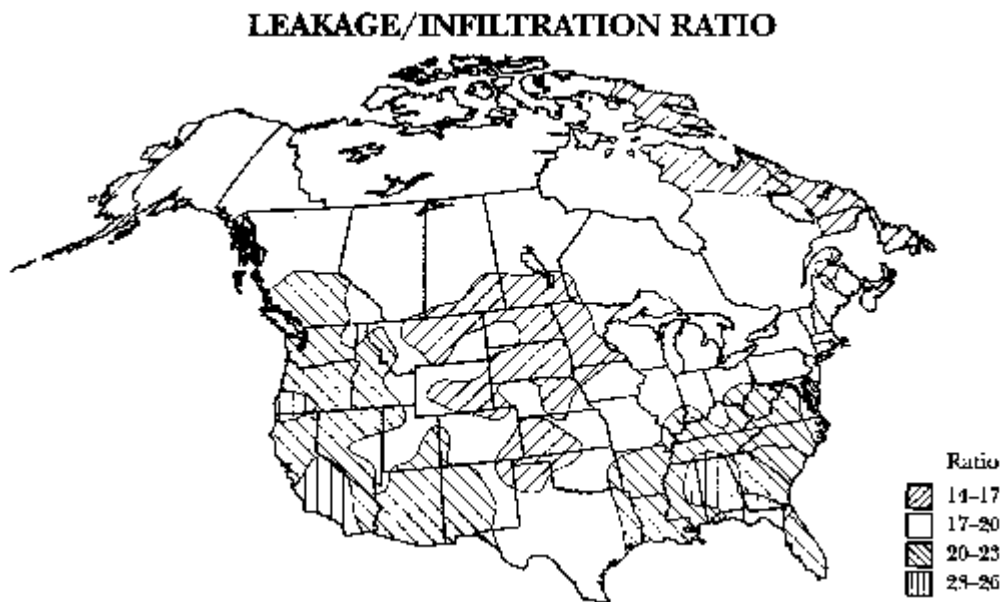
---

**Table 3. Leakiness Correction Factor**

*Select the most appropriate value and insert in Equation 2.*

Type of holes	small cracks (tight)	normal	large holes (loose)
Correction factor "L"	1.4	1.0	0.7



**Figure 1: LEAKAGE/INFILTRATION RATIO**

Climate correction factor, "C," for calculating average infiltration rates in North America. Note that the climate correction factor depends on both average temperatures and windiness. It also includes possible air infiltration during the cooling season. For these reasons, locations in greatly dissimilar climates, such as Texas and Vermont, can have equal factors. Select the value nearest to the house's location and insert it in Equation 2. This map is based on data from 250 weather stations.

## Appendix F Calculating a Design Air Infiltration Rate

The following procedure can be used to calculate a design air infiltration rate for a house from a single or multi-point blower door airtightness test. Calculated design air infiltration rates can be used in ACCA Manual J load calculations in lieu of the estimation procedures listed in Manual J. The calculation procedure presented below is based on the Lawrence Berkeley Laboratory (LBL) infiltration model. More information on this procedure can be found in the 2009 ASHRAE Fundamentals Handbook, Section 27.21.

**Note:** This calculation procedure is contained in the TECTITE test analysis software.

- Determine the 4 Pascal Effective Leakage Area (ELA) of the house in square inches from the Blower Door test data. This can be done in 2 ways:
  1. Perform a multi-point Blower Door test of the house and determine the ELA using the TECTITE software, or
  2. Perform a single-point 50 Pa Blower Door test to determine house CFM50. Multiply CFM50 by 0.055 to estimate the ELA of the house in square inches. This procedure assumes the "House Leakage Curve" has a slope (or "N" value) of 0.65. Research has shown that  $N = 0.65$  is a reasonable assumption for a large sample of houses.
- Determine the *Stack Coefficient (A)* and the *Wind Coefficient (B)* for the house from the Tables below:

### *Stack Coefficient (A)*

<u>House Height (Stories)</u>		
<u>One</u>	<u>Two</u>	<u>Three</u>
0.0150	0.0299	0.0449

### *Wind Coefficient (B)*

<u>Shielding Class</u>	<u>House Height (Stories)</u>		
	<u>One</u>	<u>Two</u>	<u>Three</u>
1	0.0119	0.0157	0.0184
2	0.0092	0.0121	0.0143
3	0.0065	0.0086	0.0101
4	0.0039	0.0051	0.0060
5	0.0012	0.0016	0.0018

### Shielding Class Description

1. No obstructions or local shielding.
2. Light local shielding, few obstructions, a few trees or small shed.
3. Moderate local shielding; some obstructions within two house heights, thick hedge, solid fence or one neighboring house.
4. Heavy shielding; obstructions around most of perimeter, building or trees within 30 feet in most directions; typical suburban shielding.
5. Very heavy shielding; large obstructions surrounding perimeter within two house heights; typical downtown shielding.

- Determine the air flow rate due to infiltration from the following equation:

$$Q = L \times ((A \times T) + (B \times V^2))^{1/2}$$

where:

Q = airflow rate in cubic feet per minute (CFM).

L = Effective Leakage Area (ELA) in square inches.

A = Stack Coefficient.

T = Design indoor-outdoor temperature difference (F).

B = Wind Coefficient.

V = Design wind speed (MPH - measured at a local weather station).

Frequency data for mean hourly wind speeds within the United States can be found in a summarized printed pamphlet from the National Climatic Center in Asheville, North Carolina, and from the Atmospheric Environment Service in Downsview, Ontario for Canadian sites.

- Convert airflow rate in CFM to Air Changes per Hour (ACH).

$$ACH = (Q \times 60) / \text{Volume of House in Cubic Feet}$$

### **Example Calculation**

Estimate the winter-time design infiltration rate for a 2 story, 30,000 cubic foot house in Minneapolis with suburban wind shielding. Use a design wind speed of 20 MPH and a design temperature difference of 82 degrees F. A single-point Blower Door test of the house measured an airtightness rate of 2,350 CFM50.

$$\text{Estimated ELA in square inches} = 2,350 \times 0.055 = 129.25$$

$$Q = 129.25 \times ((0.0313 \times 82) + (0.0051 \times 20^2))^{1/2}$$

$$= 277.4 \text{ CFM}$$

$$ACH = (277.4 \times 60) / 30,000 = 0.55 \text{ ACH}$$

## Appendix G References

1. ASHRAE, 1989. ASHRAE Standard 62-1989, "Ventilation for Acceptable Indoor Air Quality." American Society of Heating, Refrigerating and Air-Conditioning Engineers, Inc.
2. ASTM, 1987. ASTM Standard E779-87, "Standard Test Method for Determining Air Leakage Rate by Fan Pressurization" American Society for Testing and Materials.
3. Canadian General Standards Board, 1986. "Determining of the Airtightness of Building Envelopes by the Fan Depressurization Method" Standard CAN/CGSB-149.10-M86.
4. CMHC, 1988. "Chimney Safety Tests Users' Manual: Procedures for Determining the Safety of Residential Chimneys." Canada Mortgage and Housing Corporation Information Centre, 700 Montreal Rd., Ottawa, Ontario, Canada K1A-0P7 (613) 748-2000.
5. ASHRAE, 1988. ASHRAE Standard 119-1988, "Air Leakage Performance for Detached Single-Family Residential Buildings." American Society of Heating, Refrigerating and Air-Conditioning Engineers, Inc.
6. ASHRAE, 1993. ASHRAE Standard 136-1993. "A Method of Determining Air Change Rates in Detached Dwellings." American Society of Heating, Refrigeration and Air-Conditioning Engineers, Inc.
7. Cummings, James, Tooley, John and Moyer, Neil, 1991. "Investigation of Air Distribution System Leakage and It's Impact in Central Florida Homes" Florida Solar Energy Center, January 1991.
8. Fitzgerald, Jim, Nelson, Gary and Shen, Lester, 1990. "Sidewall Insulation and Air Leakage Control" Home Energy, January/February 1990. pp 13-20.
9. Meier, Alan, 1986. "Infiltration: Just ACH50 Divided By 20?" Energy Auditor and Retrofitter (now Home Energy), July/August 1986. pp 16-19.
10. Moffatt, Sebastian, 1990. "Backdrafting Causes and Cures" Journal of Light Construction, 1990. pp. 27-29.
11. Palmiter, Larry, Brown, Ian and Bond, Tammi, 1990. "Infiltration and Ventilation in New Electrically Heated Homes in the Pacific Northwest" Proceedings of the ACEEE 1990 Summer Study on Energy Efficiency in Buildings, Volume 9. pp 9.241-9.252.
12. Shen, Lester, Nelson, Gary, Dutt, Gautam and Esposito, Bonnie, 1990. "Cost-Effective Weatherization in Minnesota: The M200 Enhanced Low-Income Weatherization" Energy Exchange, August 1990. pp 13-18.
13. Tooley, John and Moyer, Neil, 1989. "Air Handler Fan: A Driving Force for Air Infiltration" Home Energy, November/December 1989. pp 11-15.
14. Tooley, John and Moyer, Neil, 1989. "MAD-AIR" Residential Energy Forum (now Southern Comfort), Summer 1989. pp 2-3, 9.
15. Tooley, John and Moyer, Neil, 1990. "Duct Busting" Southern Comfort, August 1990. pp 2-4, 5, 8.
16. Tooley, John, Moyer, Neil and Cummings, James, 1991. "Pressure Differential "The Measurement of a New Decade"" Proceeding of the Ninth Annual International Energy Efficiency Building Conference, Indianapolis, IN, March 91. pp A38-A52.

## Appendix H Air Density Correction Factors

### H.1 Air Density Correction Factors for Depressurization Testing

		INSIDE TEMPERATURE (F)								
		50	55	60	65	70	75	80	85	90
OUTSIDE TEMPERATURE (F)	-20	0.929	0.924	0.920	0.915	0.911	0.907	0.903	0.898	0.894
	-15	0.934	0.930	0.925	0.921	0.916	0.912	0.908	0.904	0.899
	-10	0.939	0.935	0.930	0.926	0.921	0.917	0.913	0.909	0.904
	-5	0.945	0.940	0.935	0.931	0.927	0.922	0.918	0.914	0.909
	0	0.950	0.945	0.941	0.936	0.932	0.927	0.923	0.919	0.914
	5	0.955	0.950	0.946	0.941	0.937	0.932	0.928	0.924	0.919
	10	0.960	0.955	0.951	0.946	0.942	0.937	0.933	0.929	0.924
	15	0.965	0.960	0.956	0.951	0.947	0.942	0.938	0.934	0.929
	20	0.970	0.965	0.961	0.956	0.952	0.947	0.943	0.938	0.934
	25	0.975	0.970	0.966	0.961	0.957	0.952	0.948	0.943	0.939
	30	0.980	0.975	0.971	0.966	0.962	0.957	0.953	0.948	0.944
	35	0.985	0.980	0.976	0.971	0.966	0.962	0.957	0.953	0.949
	40	0.990	0.985	0.981	0.976	0.971	0.967	0.962	0.958	0.953
	45	0.995	0.990	0.985	0.981	0.976	0.972	0.967	0.963	0.958
	50	1.000	0.995	0.990	0.986	0.981	0.976	0.972	0.967	0.963
	55	1.005	1.000	0.995	0.990	0.986	0.981	0.977	0.972	0.968
	60	1.010	1.005	1.000	0.995	0.991	0.986	0.981	0.977	0.972
	65	1.015	1.010	1.005	1.000	0.995	0.991	0.986	0.981	0.977
	70	1.019	1.014	1.010	1.005	1.000	0.995	0.991	0.986	0.982
	75	1.024	1.019	1.014	1.009	1.005	1.000	0.995	0.991	0.986
	80	1.029	1.024	1.019	1.014	1.009	1.005	1.000	0.995	0.991
	85	1.034	1.029	1.024	1.019	1.014	1.009	1.005	1.000	0.995
	90	1.038	1.033	1.028	1.024	1.019	1.014	1.009	1.005	1.000
	95	1.043	1.038	1.033	1.028	1.023	1.019	1.014	1.009	1.005
	100	1.048	1.043	1.038	1.033	1.028	1.023	1.018	1.014	1.009
	105	1.053	1.047	1.042	1.037	1.033	1.028	1.023	1.018	1.014
	110	1.057	1.052	1.047	1.042	1.037	1.032	1.027	1.023	1.018

To use the air density correction factor, multiply the measured fan flow by the appropriate correction factor from the Table above. For example, if the measured fan flow was 3,200 cfm, and during the test the inside temperature was 70 F and the outside temperature was 40 F, the appropriate correction factor would be 0.971. The density corrected fan flow is  $3,200 \times 0.971 = 3,107$  cfm

## H.2 Air Density Correction Factors for Pressurization Testing

		INSIDE TEMPERATURE (F)								
		50	55	60	65	70	75	80	85	90
OUTSIDE TEMPERATURE (F)	-20	1.077	1.082	1.087	1.092	1.098	1.103	1.108	1.113	1.118
	-15	1.071	1.076	1.081	1.086	1.091	1.097	1.102	1.107	1.112
	-10	1.065	1.070	1.075	1.080	1.085	1.090	1.096	1.101	1.106
	-5	1.059	1.064	1.069	1.074	1.079	1.084	1.089	1.095	1.100
	0	1.053	1.058	1.063	1.068	1.073	1.078	1.084	1.089	1.094
	5	1.047	1.052	1.058	1.063	1.068	1.073	1.078	1.083	1.088
	10	1.042	1.047	1.052	1.057	1.062	1.067	1.072	1.077	1.082
	15	1.036	1.041	1.046	1.051	1.056	1.061	1.066	1.071	1.076
	20	1.031	1.036	1.041	1.046	1.051	1.056	1.061	1.066	1.070
	25	1.025	1.030	1.035	1.040	1.045	1.050	1.055	1.060	1.065
	30	1.020	1.025	1.030	1.035	1.040	1.045	1.050	1.055	1.059
	35	1.015	1.020	1.025	1.030	1.035	1.040	1.044	1.049	1.054
	40	1.010	1.015	1.020	1.025	1.030	1.034	1.039	1.044	1.049
	45	1.005	1.010	1.015	1.020	1.024	1.029	1.034	1.039	1.044
	50	1.000	1.005	1.010	1.015	1.019	1.024	1.029	1.034	1.038
	55	0.995	1.000	1.005	1.010	1.014	1.019	1.024	1.029	1.033
	60	0.990	0.995	1.000	1.005	1.010	1.014	1.019	1.024	1.028
	65	0.986	0.990	0.995	1.000	1.005	1.009	1.014	1.019	1.024
	70	0.981	0.986	0.991	0.995	1.000	1.005	1.009	1.014	1.019
	75	0.976	0.981	0.986	0.991	0.995	1.000	1.005	1.009	1.014
	80	0.972	0.977	0.981	0.986	0.991	0.995	1.000	1.005	1.009
	85	0.967	0.972	0.977	0.981	0.986	0.991	0.995	1.000	1.005
	90	0.963	0.968	0.972	0.977	0.982	0.986	0.991	0.995	1.000
	95	0.959	0.963	0.968	0.973	0.977	0.982	0.986	0.991	0.995
	100	0.954	0.959	0.964	0.968	0.973	0.977	0.982	0.987	0.991
	105	0.950	0.955	0.959	0.964	0.969	0.973	0.978	0.982	0.987
	110	0.946	0.951	0.955	0.960	0.964	0.969	0.973	0.978	0.982

To use the air density correction factor, multiply the measured fan flow by the appropriate correction factor from the Table above. For example, if the measured fan flow was 3,200 cfm, and during the test the inside temperature was 70 F and the outside temperature was 40 F, the appropriate correction factor would be 1.030. The density corrected fan flow is  $3,200 \times 1.030 = 3,296$  cfm.


## Appendix I Cruise Control with the DG-700 Gauge

All new DG-700 gauges include a Cruise Control feature which allows you to automatically control the Blower Door fan to maintain a constant 75 Pa, 50 Pa, 25 Pa or 0 Pa building pressure without having the gauge connected to a computer. Common applications of the Cruise Control feature include:



- Quickly measuring building airtightness using a “one-point” 50 Pa test.
- Maintaining a constant 25 Pa building pressure while conducting a “duct leakage to outside” test with a Duct Blaster system.
- Pressure pan testing for evaluating leakage in forced air duct systems.
- Maintaining a constant building pressure while locating and sealing air leaks.
- Performing series leakage to quantify leakage rates between various zones within a building.

In order to use the Cruise Control feature you will need the following 3 items:

- A “Cruise compatible” DG-700 gauge. Your DG-700 is compatible with Cruise Control if the CONFIG, CLEAR, START, and ENTER keys have additional red lettering below the main black script.
- A Blower Door fan speed controller with a 3.5 mm communication jack on the side of the controller box.
- A fan control cable to connect the DG-700 fan control jack to the speed controller communication jack.

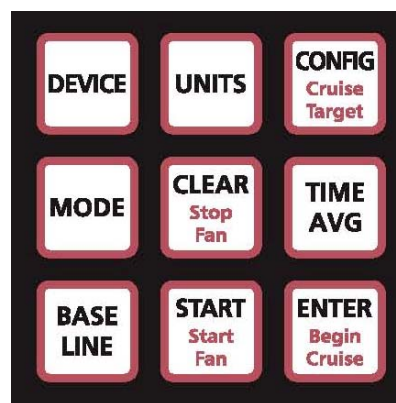

Fan Control cable with Blower Door controller

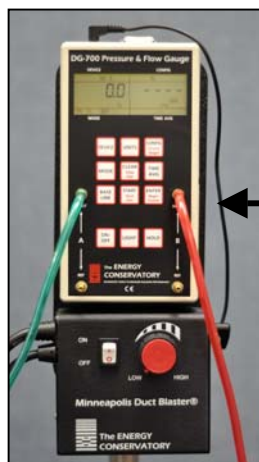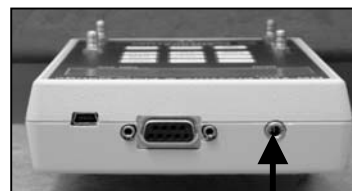

Fan control cable with Duct Blaster controller.



Fan control jacks.



## Cruise Overview

Cruise Control uses the DG-700's fan control feature to continuously adjust the (Blower Door) fan to maintain a constant Cruise target pressure on **Channel A** of the gauge. Cruise Control can be used in the following gauge Modes to maintain the listed target pressures:

Gauge Mode	Cruise Target Pressures Available
PR/ FL @50	50 Pa
PR/ FL @25	25 Pa
PR/ FL	75 Pa, 50 Pa, 25 Pa, +0, -0
PR/ PR	75 Pa, 50 Pa, 25 Pa, +0, -0

Before starting Cruise, the Blower Door and DG-700 should be completely set-up (including tubing connections), the gauge should be in the Mode you wish to use, and the correct Device and Configuration settings should be entered. If you wish to Cruise with a baseline pressure adjustment applied to **Channel A**, simply use the Baseline feature first before beginning Cruise. You will also need to install the fan control cable and turn the Blower Door speed control knob to the "just on" position:

- Model 3 Blower Door "just on" - from the off position, turn the controller knob clockwise only until you feel the click and no farther - the fan will not be turning.
- Duct Blaster "just on" – turn the controller knob all the way down (counter-clockwise) and flip the on/off switch to "ON" – the fan will not be turning.

**Begin Cruise button:** When you are ready to begin Cruise, press **Begin Cruise** to enter Cruise setup. A Cruise target pressure will appear in the **Channel A** display and the Cruise icon will flash. The flashing Cruise icon indicates that the gauge is ready to begin Cruising but is not yet controlling the fan. If you are in the **PR/ FL** or **PR/ PR** modes, you may change the Cruise target pressure at this point by pressing the **Cruise Target** button. **Note:** You can not change the Cruise target pressure when in the **PR/ FL @50** and **PR/ FL @25** modes.

**Start Fan button:** Press **Start Fan** to instruct the DG-700 to begin ramping up the fan to achieve the target pressure on **Channel A**. The fan will slowly start increasing speed until the pressure reading on **Channel A** matches the Cruise target pressure. The fan will simply run at full speed if the target pressure can not be achieved. Whenever the DG-700 is calling for full fan speed, the gauge will emit a beeping sound.

**Stop Fan button:** Press **Stop Fan** to turn off the fan when you are done Cruising. When the fan is turned off by pressing **Stop Fan**, the DG-700 returns to the Cruise setup state (i.e. the Cruise icon is flashing and a Cruise target pressure is displayed on **Channel A**). You may re-start Cruise again by pressing **Start Fan**, or exit the Cruise feature altogether by pressing the **CLEAR** button.

The fan will also be stopped while Cruising under the following circumstances:

- If **Channel A** registers a pressure of 100 Pa or more, the fan will automatically be shut down and the gauge will revert back to the Cruise setup state.
- Pressing the **HOLD** button will shut down the fan and freeze the display. Pressing **Start Fan** from a display freeze will re-start Cruise. Pressing the **HOLD** button a second time from a display freeze will return the gauge to the Cruise setup state.
- The DG-700's auto-off feature will shut down the gauge and turn off the fan after 2 hours of run-time (if no buttons are pressed during that time).

## Cruising Zero (+0 and -0)

Cruising Zero is designed for specialized testing/research applications and will typically not be used by most Blower Door technicians. Cruising Zero is useful if you want to control the Blower Door fan to remove an existing pressure from a building or other enclosure. When using the fan to pressurize a space (that is currently depressurized) use +0 as your Cruise target pressure. When using the fan to depressurize a space (that is currently pressurized), use -0 as the Cruise target pressure.

## Appendix J Blower Door System Specifications

**Maximum Flow:** (Model 3 Fan): 6,100 CFM (free air), 5,250 CFM (at 50 Pa).  
(Model 4 Fan): 4,850 CFM (free air), 4,320 CFM (at 50 Pa).

**Minimum Flow:** 300 CFM (Ring B), 85 CFM (Ring C), 30 CFM (Ring D), 11 CFM (Ring E).

**Flow Accuracy:** +/- 3% with DG-500, DG-700 (+/- 4% or 1 CFM for Rings D & E).

**Calibration:** Meets ASTM Standard E779-10, E1554-07, CGSB-149.10-M86, RESNET 2012, EN 13829, CIBSE TM23, ATTMA TS-1 and NFPA 2001.

**Electrical Input:** (Model 3 Fan): 100-130V/60Hz, 8.5A, 1Ph.  
(Model 4 Fan): 220-240V/50Hz, 3.7A, 1Ph.

**Fan Over-Current Protection Fuse (Model 4):** 250VAC/5AF VDE,UL Approved.

**Fan Motor Rating:** 3/4 Hp, Class B Insulation, Thermally Protected.

**Fan Control Jack Isolation Rating:** VISO > 2500 VRMS.

**Operational Environment:** 0 to 48 degree C, 10-90% R.H. (non-condensing).

**Dimensions:** (Fan): 20 in. inlet diameter, 10.25 in. length.  
(Frame): 28 in. to 40 in. width, 52 in. to 96 in. height (adjustable).

**Weight:** 33 lbs. (15 kg) with Rings A & B.

### Options:

**DG-700 Gauge Universal AC Adapter:** 100-240V/50-60Hz Input, 12 VDC Output, Center "+", 12mm Barrel Length, 3W Min. Output (International mains adapters included).